

Sample Name: LAH4
 Cat. No. : RP20096
 Lot. No. : E3153919H
 Time Processed :7:23:56
 Month-Day-Year Processed :08/22/2019
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GR1101009

Chromatogram

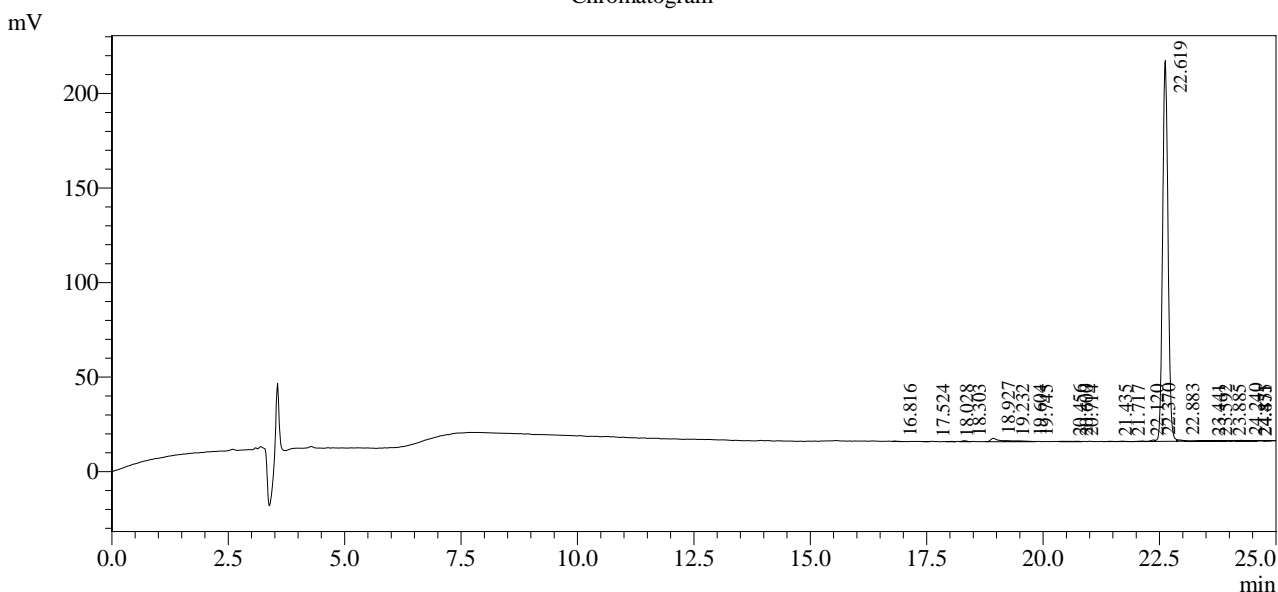

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	16.816	981	199	0.057
2	17.524	1132	164	0.066
3	18.028	1186	199	0.069
4	18.303	4385	569	0.257
5	18.927	21230	1812	1.243
6	19.232	8212	580	0.481
7	19.604	4494	423	0.263
8	19.745	1296	224	0.076
9	20.456	1919	258	0.112
10	20.600	1375	182	0.080
11	20.714	1687	249	0.099
12	21.435	1478	178	0.087
13	21.717	2244	223	0.131
14	22.120	2787	293	0.163
15	22.370	5097	753	0.298
16	22.619	1633694	201437	95.634
17	22.883	3883	748	0.227
18	23.441	1866	270	0.109
19	23.592	1254	190	0.073
20	23.885	1283	232	0.075
21	24.240	4146	391	0.243
22	24.455	1508	186	0.088
23	24.871	1147	143	0.067
Total		1708283	209904	100.000