

Sample Name :Neuropeptide Y, human
 Cat No. :RP10492
 Lot No. :PE9361901
 Time Processed :9:41:42
 Month-Day-Year Processed :01/11/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

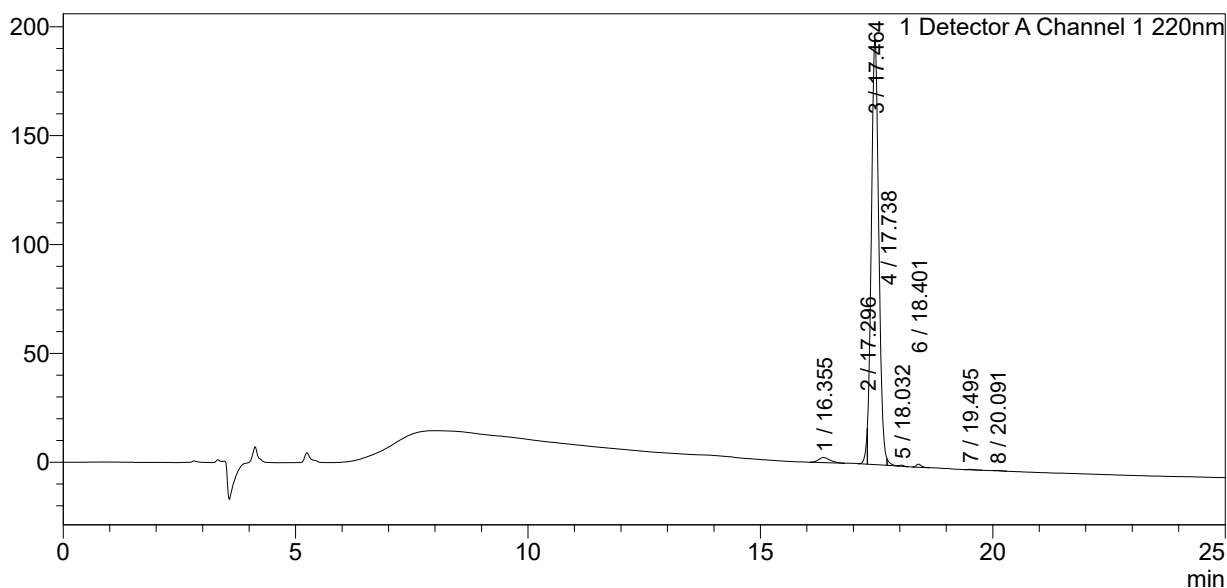

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.355	41307	2377	1.812
2	17.296	40838	13373	1.791
3	17.464	2171822	195323	95.261
4	17.738	9610	2523	0.422
5	18.032	2726	470	0.120
6	18.401	10277	1431	0.451
7	19.495	1839	207	0.081
8	20.091	1441	152	0.063
Total		2279859	215855	100.000