

Sample Name :DYKDDDDK Peptide
 Cat No. :RP10586
 Lot No. :E0657021A
 Time Processed :1:20:22 PM
 Month-Day-Year Processed :02/01/21

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	0
5.00	Pumps	B.Conc	0
20.00	Pumps	B.Conc	30
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	0
40.00	Pumps	B.Conc	0
40.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ17010508

<Chromatogram>

mV

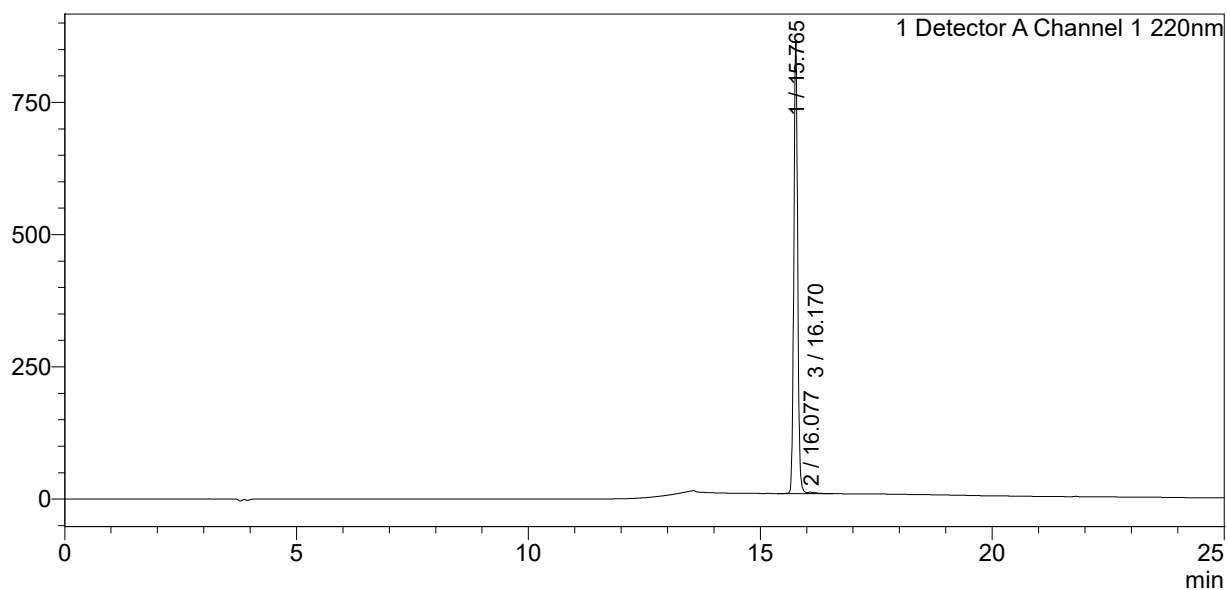

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.765	4951659	857877	99.354
2	16.077	18769	2795	0.377
3	16.170	13418	2118	0.269
Total		4983846	862789	100.000