

Sample Name :OVA Peptide (323-339)
 Cat No. :RP10610
 Lot No. :E5112320F
 Time Processed :1:12:34 PM
 Month-Day-Year Processed :06/10/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>
 Column : Alltima™ C18 4.6 x 250 mm
 Equipment:ZJ19010141

<Chromatogram>

mV

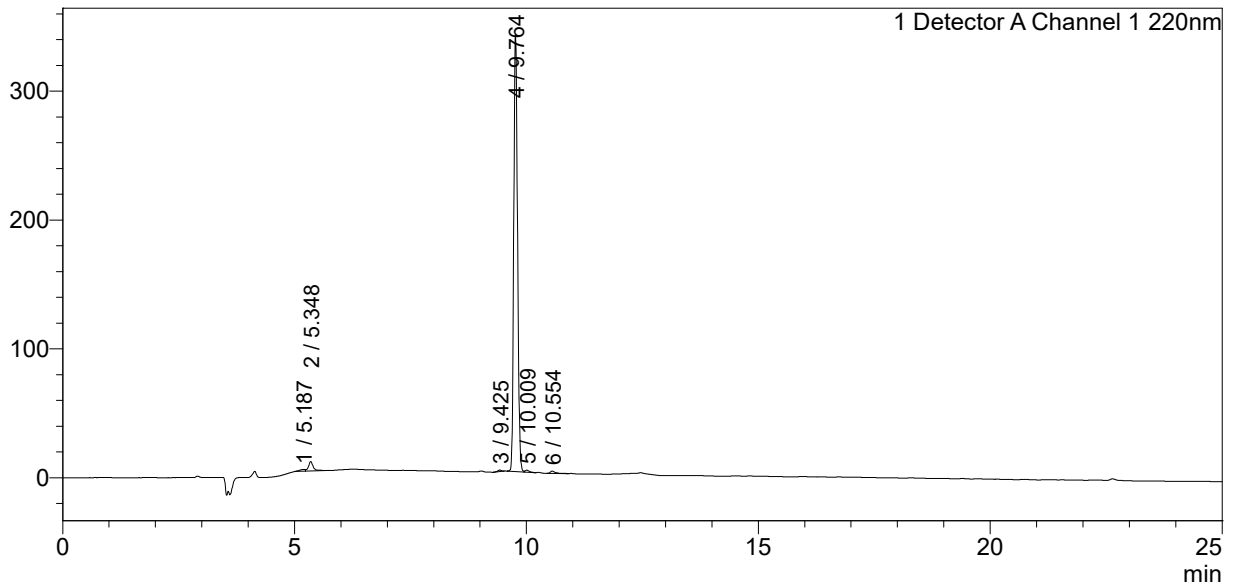

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.187	11770	1305	0.586
2	5.348	54270	7372	2.704
3	9.425	6507	1190	0.324
4	9.764	1911269	339653	95.239
5	10.009	9765	1544	0.487
6	10.554	13237	1809	0.660
Total		2006818	352873	100.000