

Sample Name : OVA Peptide (323-339)  
 Cat. No. : RP10610  
 Lot. No. : E5559220A  
 Time Processed :7:50:49  
 Month-Day-Year Processed :01/10/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GR11010440

Chromatogram

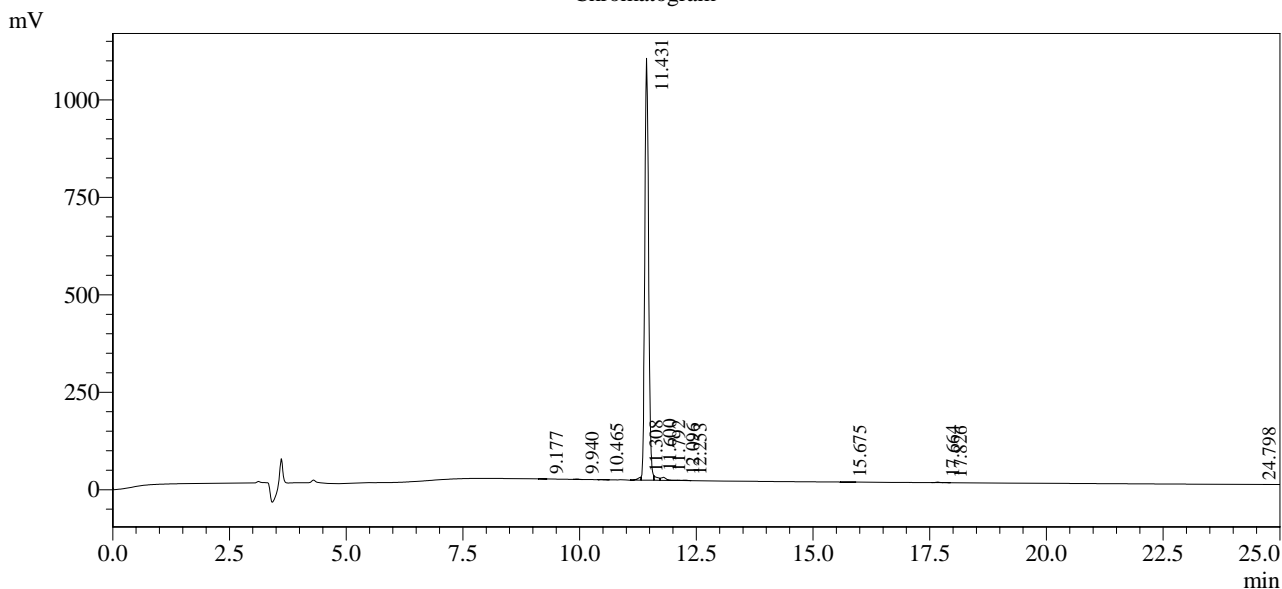

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.177	2316	506	0.036
2	9.940	5030	1016	0.079
3	10.465	2348	418	0.037
4	11.308	37203	7341	0.581
5	11.431	6207001	1082282	96.987
6	11.600	58681	10609	0.917
7	11.792	60853	7742	0.951
8	12.096	7237	950	0.113
9	12.253	6228	910	0.097
10	15.675	1599	238	0.025
11	17.664	6892	1286	0.108
12	17.826	1359	281	0.021
13	24.798	3096	358	0.048
Total		6399844	1113937	100.000