

Sample Name :OVA Peptide (323-339)
 Cat No. :RP10610
 Lot No. :E80132201
 Time Processed :11:18:36 PM
 Month-Day-Year Processed :09/26/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

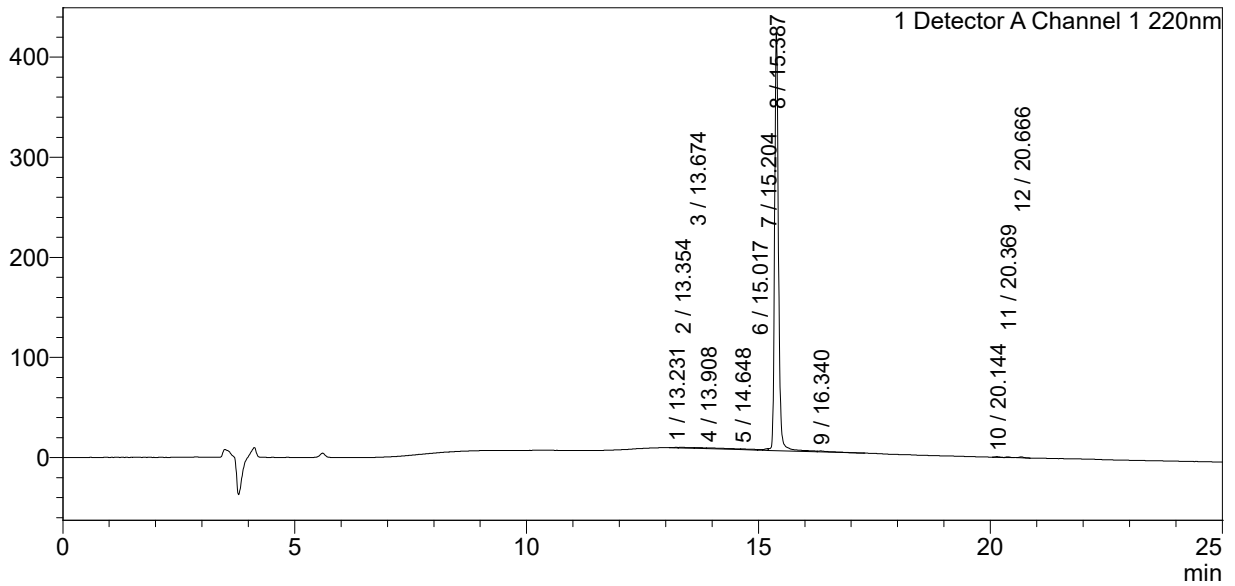

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.231	2076	308	0.081
2	13.354	10928	498	0.428
3	13.674	10992	764	0.431
4	13.908	31145	788	1.221
5	14.648	14431	648	0.566
6	15.017	4690	722	0.184
7	15.204	8965	1690	0.351
8	15.387	2433922	416643	95.406
9	16.340	20238	958	0.793
10	20.144	3829	597	0.150
11	20.369	3880	665	0.152
12	20.666	6031	930	0.236
Total		2551127	425210	100.000