

Sample Name : DYKDDDDK Peptide
 Cat. No. : RP10586
 Lot. No. : E4882920F
 Time Processed :13:57:50
 Month-Day-Year Processed :07/03/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

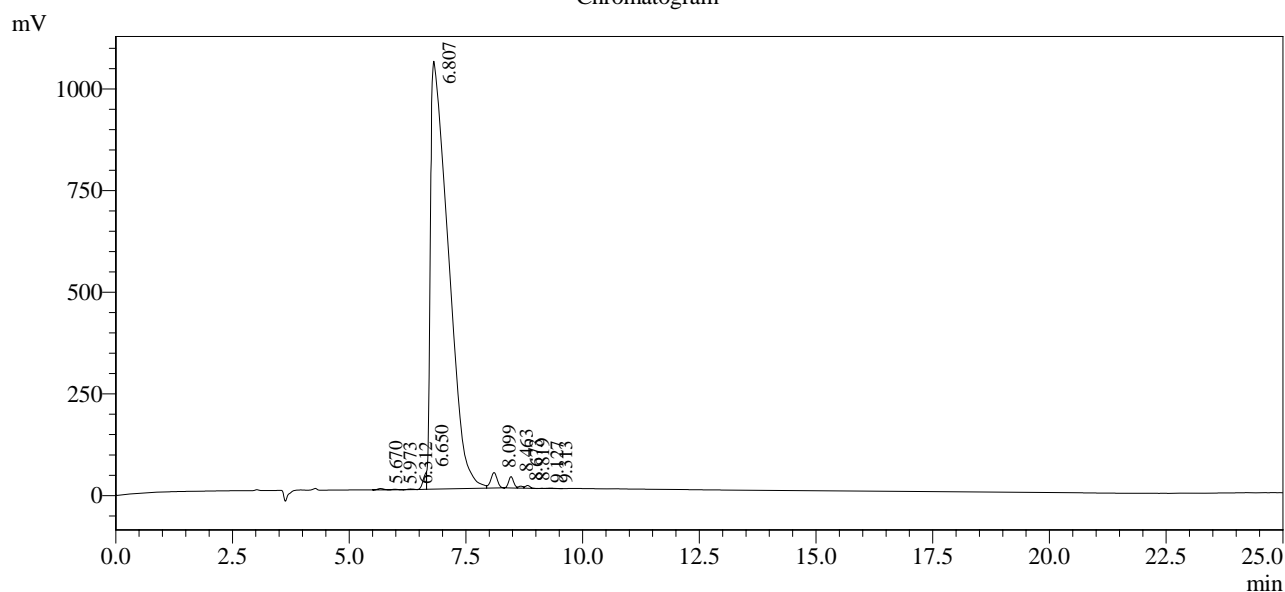

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	5.670	32056	3417	0.110
2	5.973	12142	1485	0.042
3	6.312	13419	1520	0.046
4	6.650	213381	41764	0.734
5	6.807	28137102	1052345	96.774
6	8.099	366065	37999	1.259
7	8.463	209222	28126	0.720
8	8.673	33562	4913	0.115
9	8.819	48048	6828	0.165
10	9.127	1183	203	0.004
11	9.313	8857	944	0.030
Total		29075037	1179543	100.000