

Sample Name :OVA G4 peptide
 Cat No. :RP20398
 Lot No. :E8203321C
 Time Processed :18:59:03
 Month-Day-Year Processed :03/14/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

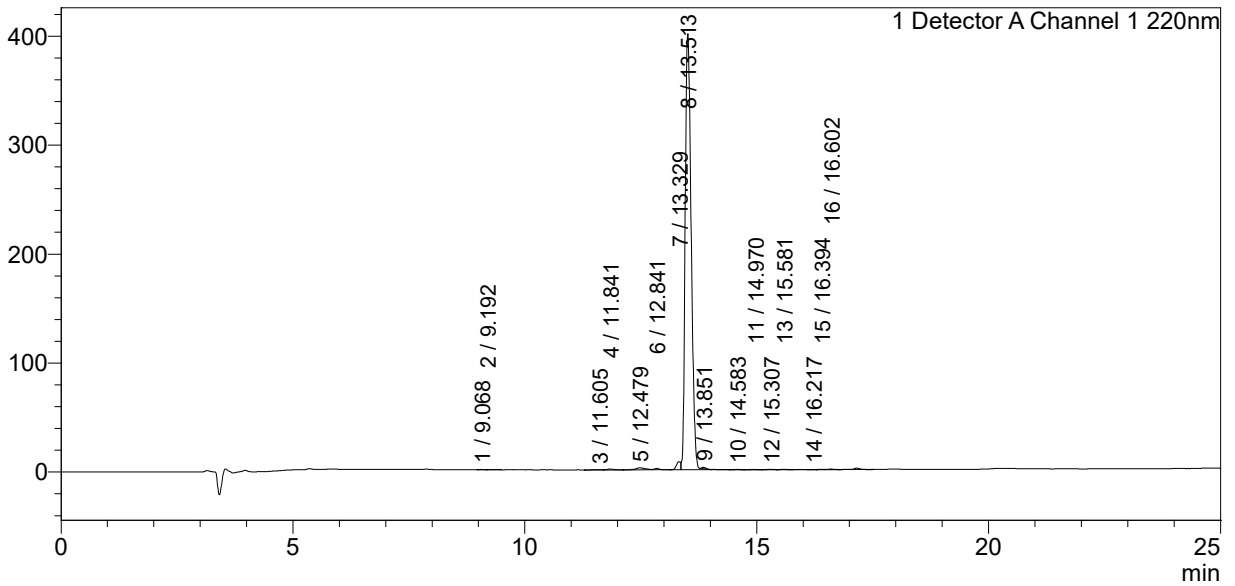

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.068	1443	173	0.039
2	9.192	1503	152	0.040
3	11.605	2762	216	0.074
4	11.841	8546	749	0.229
5	12.479	29108	1854	0.779
6	12.841	11076	1253	0.296
7	13.329	48875	7373	1.308
8	13.513	3605629	400323	96.491
9	13.851	8467	1451	0.227
10	14.583	2581	242	0.069
11	14.970	3112	176	0.083
12	15.307	4137	372	0.111
13	15.581	3887	438	0.104
14	16.217	483	59	0.013

Peak#	Ret. Time	Area	Height	Area%
15	16.394	1099	139	0.029
16	16.602	4025	399	0.108
Total		3736733	415370	100.000