


Mass Spectrum

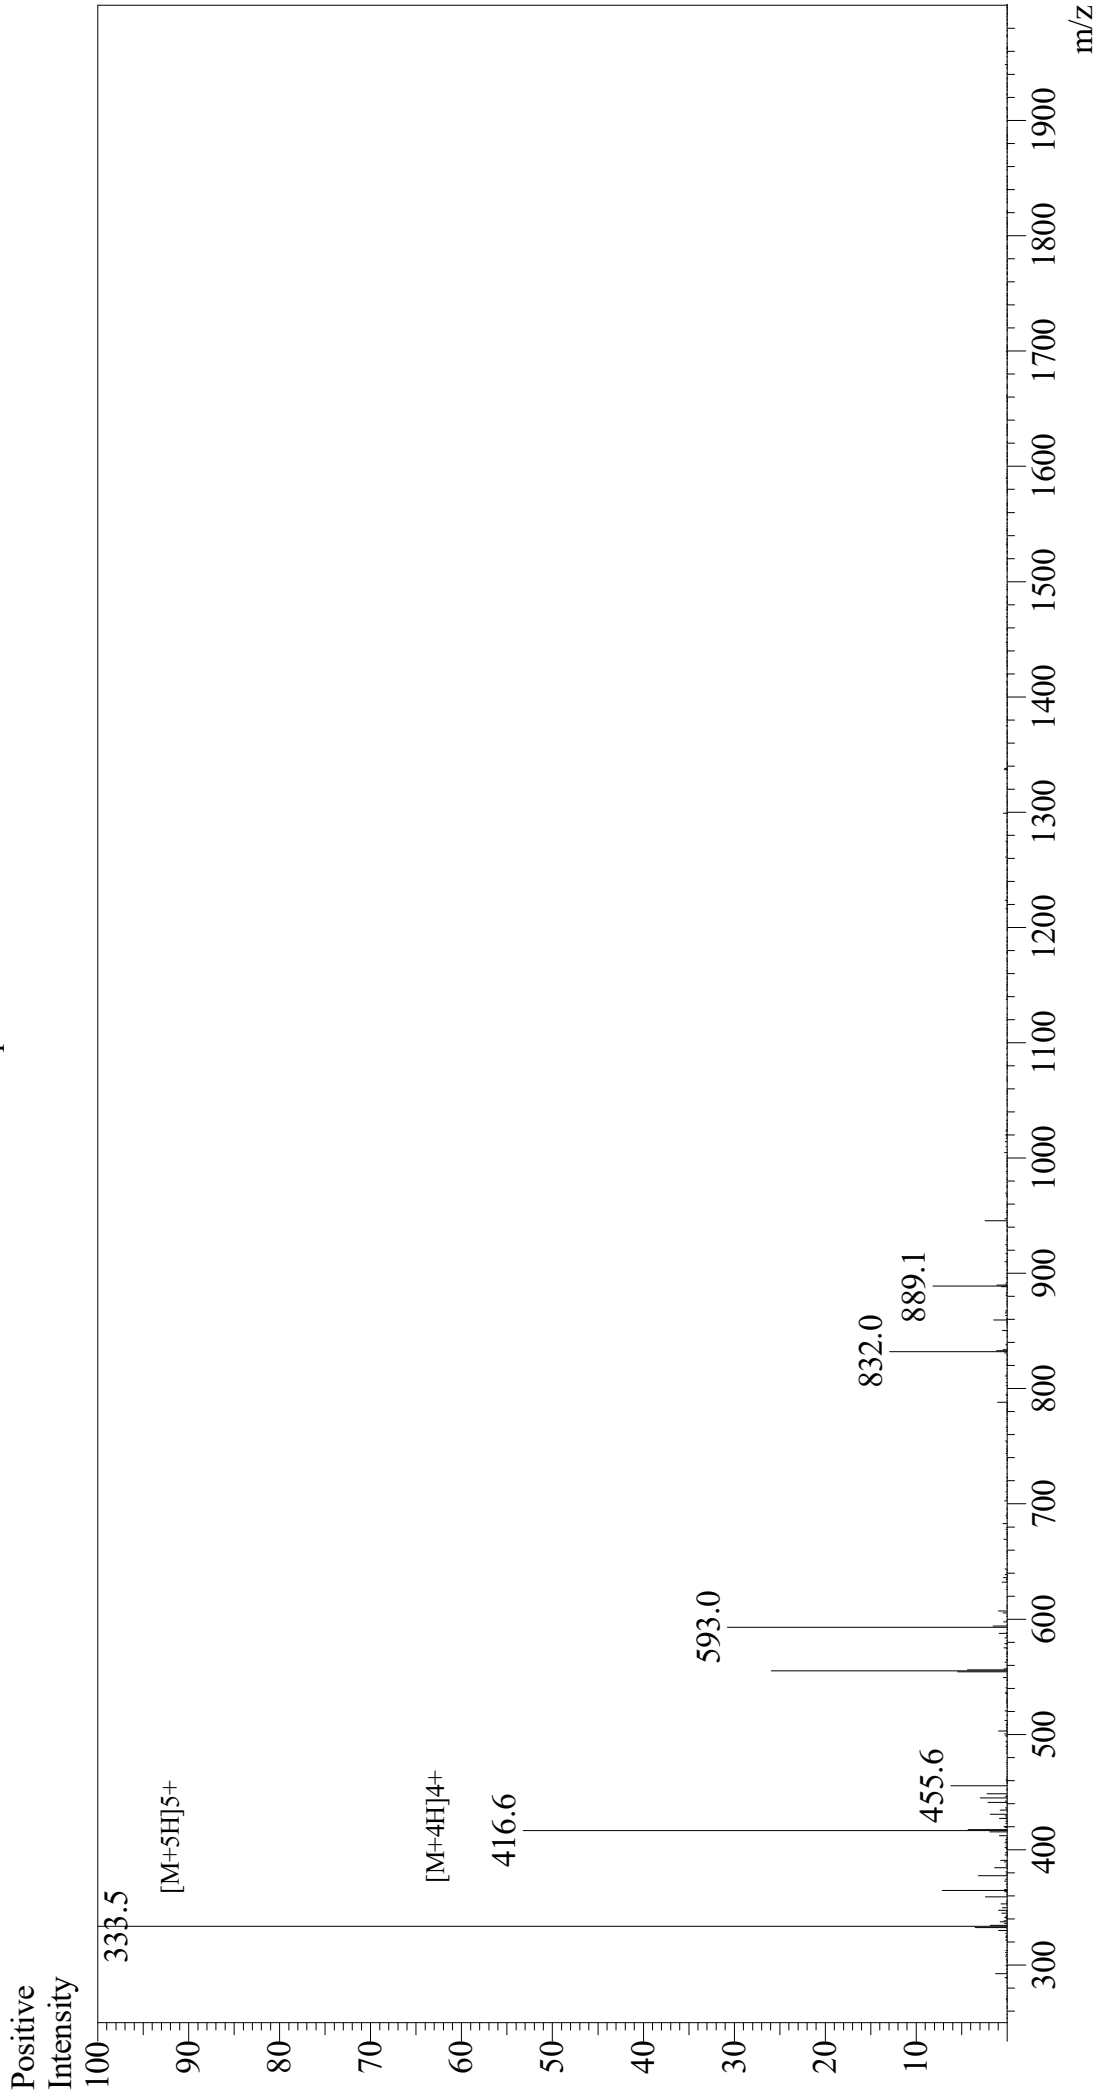

Sample Information
Month-Day Processed : 05/27/21
Time Processed : 16:30:23
Injection Volume : 0.2
Sample Name : Cys-TAT(47-57)
Cat No. : RP20343
Lot No. : E6787621E
Theoretical MW : 1661.99
Observed MW : 1662.5

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +3.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H2O/50%MeOH