

Sample Name :HA Peptide
 Cat. No. : RP11735
 Lot. No. : E4192619F
 Time Processed : 23:23:21
 Month-Day-Year Processed :06/10/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

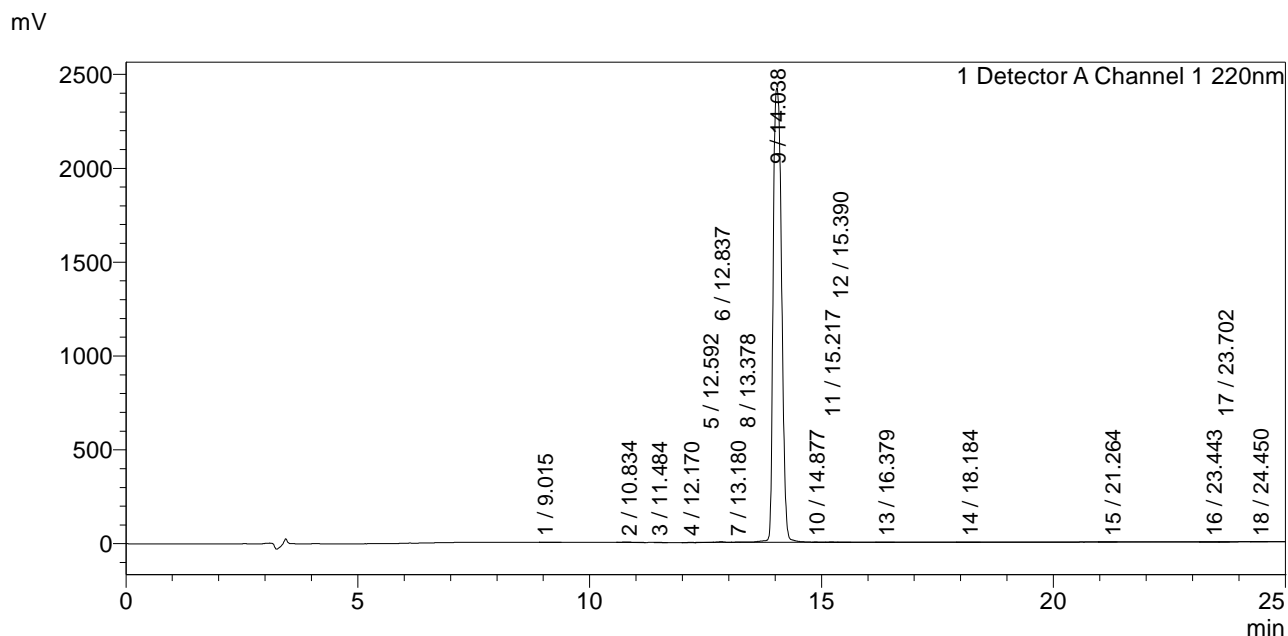

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.015	1692	148	0.006
2	10.834	33160	2649	0.110
3	11.484	3074	441	0.010
4	12.170	3248	548	0.011
5	12.592	14366	1281	0.048
6	12.837	45353	3814	0.150
7	13.180	17279	2454	0.057
8	13.378	30031	2509	0.100
9	14.038	29946711	2420609	99.376
10	14.877	4393	508	0.015
11	15.217	13641	1657	0.045
12	15.390	4046	472	0.013
13	16.379	2074	167	0.007
14	18.184	3861	288	0.013
15	21.264	1568	188	0.005

Peak#	Ret. Time	Area	Height	Area%
16	23.443	4605	315	0.015
17	23.702	1123	129	0.004
18	24.450	4510	439	0.015
Total		30134733	2438615	100.000