

Sample Name :RGD
 Cat No.: RP20297
 Lot No.: E3875220G
 Time Processed :10:47:11
 Month-Day-Year Processed :07/19/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	15
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
32.00	Pumps	Solvent B Conc.	95
32.01	Pumps	Solvent B Conc.	15
42.00	Pumps	Solvent B Conc.	15
95.00	Controller	Stop	

<<Column Performance>>

<Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

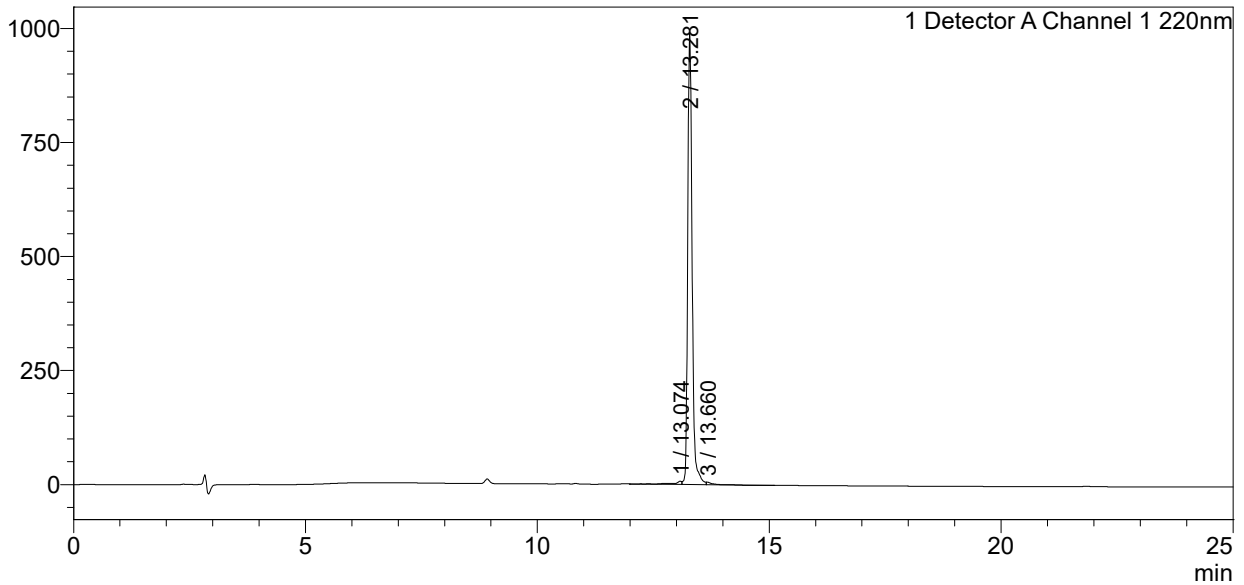

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.074	89249	7039	1.331
2	13.281	6577025	990239	98.081
3	13.660	39454	5693	0.588
Total		6705727	1002971	100.000