

Sample Name :Melittin,honey bee
 Cat No.: RP20415
 Lot No.: E0869219K
 Time Processed :15:41:15
 Month-Day-Year Processed :12/04/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
30.00	Pumps	Pump A B.Conc	95
30.10	Pumps	Pump A B.Conc	95
35.00	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
45.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

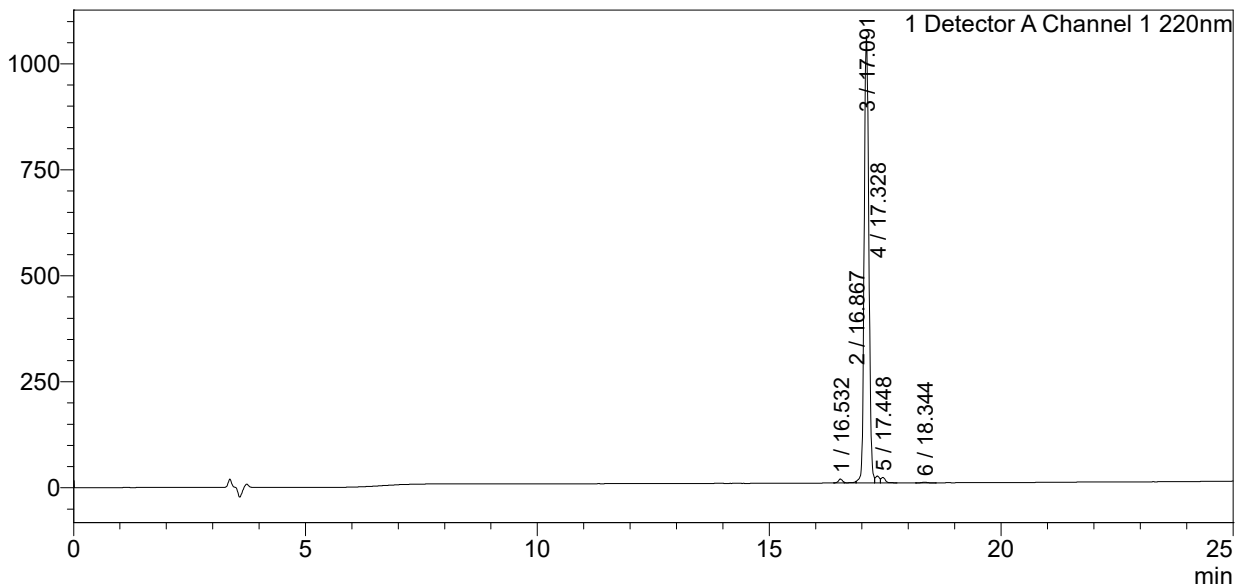

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.532	53270	9075	0.699
2	16.867	13610	3108	0.178
3	17.091	7369826	1054373	96.647
4	17.328	99922	16266	1.310
5	17.448	79060	12886	1.037
6	18.344	9799	1531	0.129
Total		7625486	1097238	100.000