

Sample Name :OVA Peptide (323-339)
 Cat No. :RP10610
 Lot No. :E4191221A
 Time Processed :4:07:04 AM
 Month-Day-Year Processed :01/31/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

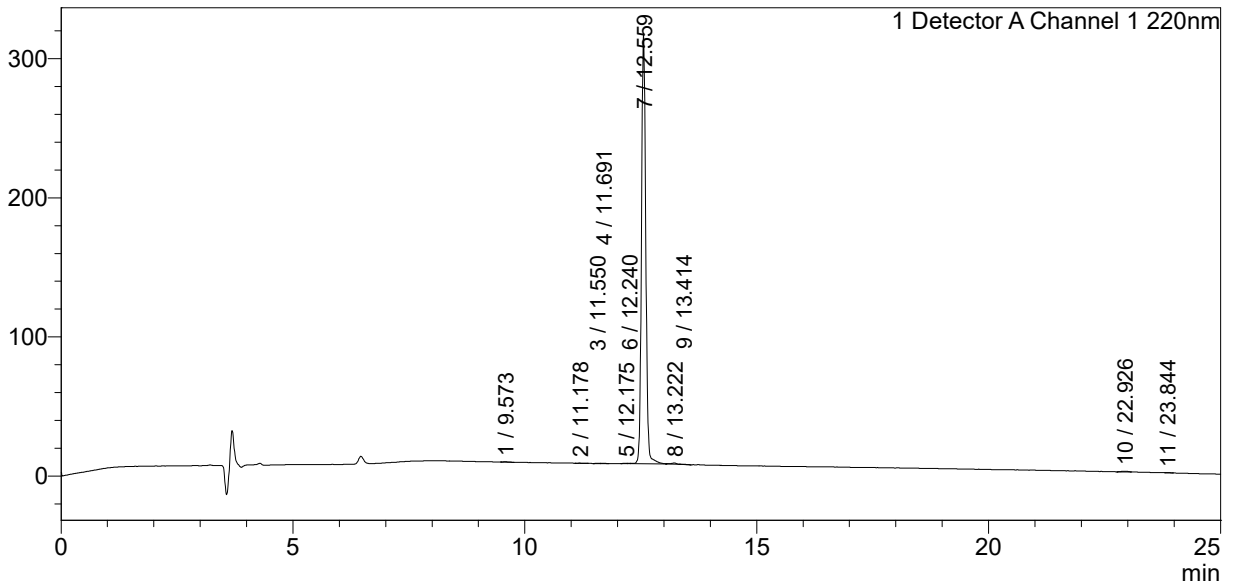

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.573	2102	274	0.104
2	11.178	1303	172	0.065
3	11.550	1109	160	0.055
4	11.691	1624	267	0.080
5	12.175	2073	286	0.103
6	12.240	1165	298	0.058
7	12.559	1998668	309043	98.946
8	13.222	5495	797	0.272
9	13.414	1055	152	0.052
10	22.926	4113	433	0.204
11	23.844	1248	215	0.062
Total		2019954	312098	100.000