

Sample Name : Calcitonin Gene Related Peptide (CGRP) (8-37), rat
 Cat. No. : RP11090
 Lot. No. : E1399919G
 Time Processed : 7:44:55
 Month-Day-Year Processed : 07/26/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

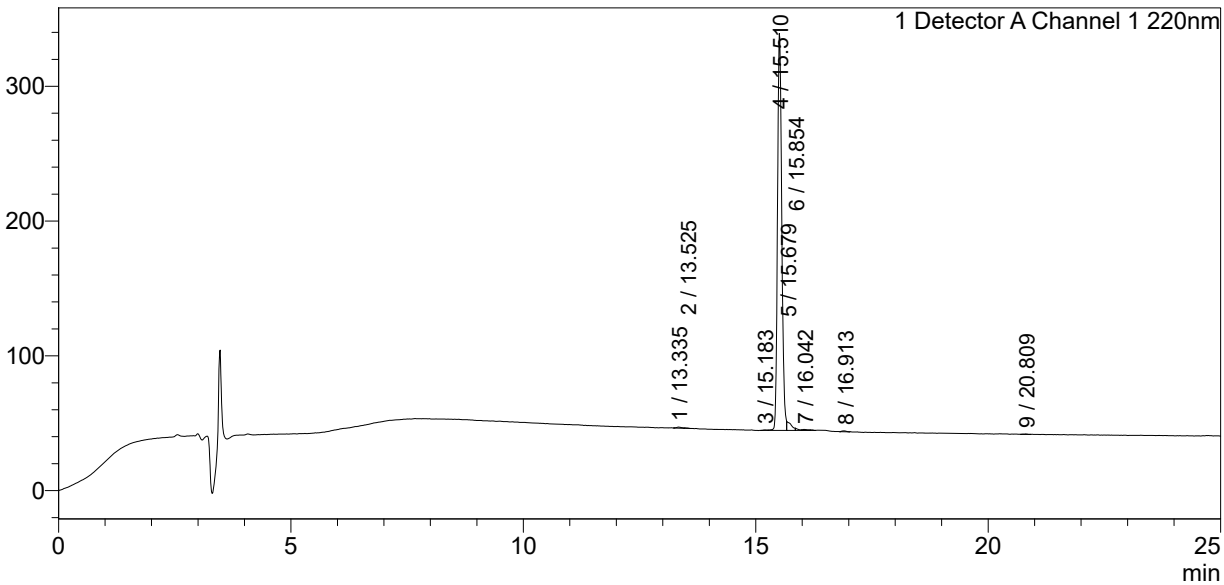

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.335	5747	745	0.297
2	13.525	1855	269	0.096
3	15.183	2198	343	0.113
4	15.510	1866954	294478	96.396
5	15.679	42758	6337	2.208
6	15.854	8146	1590	0.421
7	16.042	3130	482	0.162
8	16.913	4110	622	0.212
9	20.809	1866	333	0.096
Total		1936764	305200	100.000