

Sample Name :Chemerin-9 (149-157)
 Cat. No. : RP20248
 Lot. No. : PE8811812
 Time Processed : 12:53:44
 Month-Day-Year Processed : 12/07/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

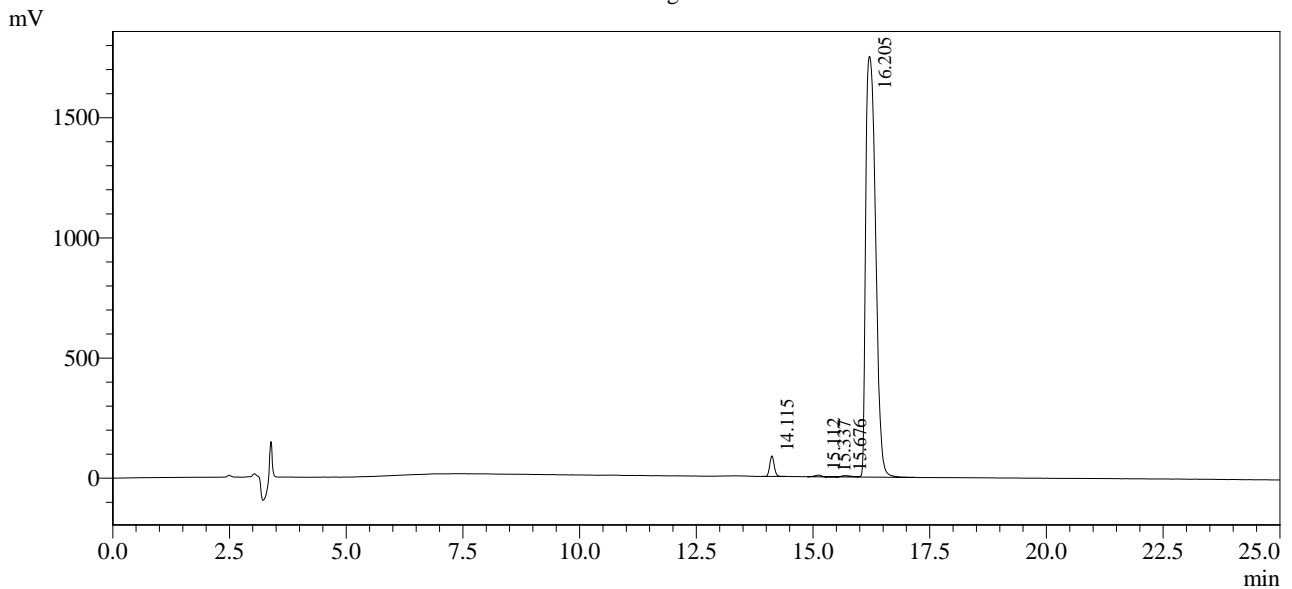

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.115	572558	85687	2.166
2	15.112	66655	6757	0.252
3	15.337	1863	336	0.007
4	15.676	85926	5520	0.325
5	16.205	25710631	1751295	97.250
Total		26437634	1849596	100.000