

Sample Name : Calcitonin Gene Related Peptide (CGRP) (8-37), rat
 Cat. No. : RP11090
 Lot. No. : E5443219H
 Time Processed : 8:08:09
 Month-Day-Year Processed : 08/17/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow : 1 ml/min
 Wavelength : 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment : SS-CM-0310

Chromatogram

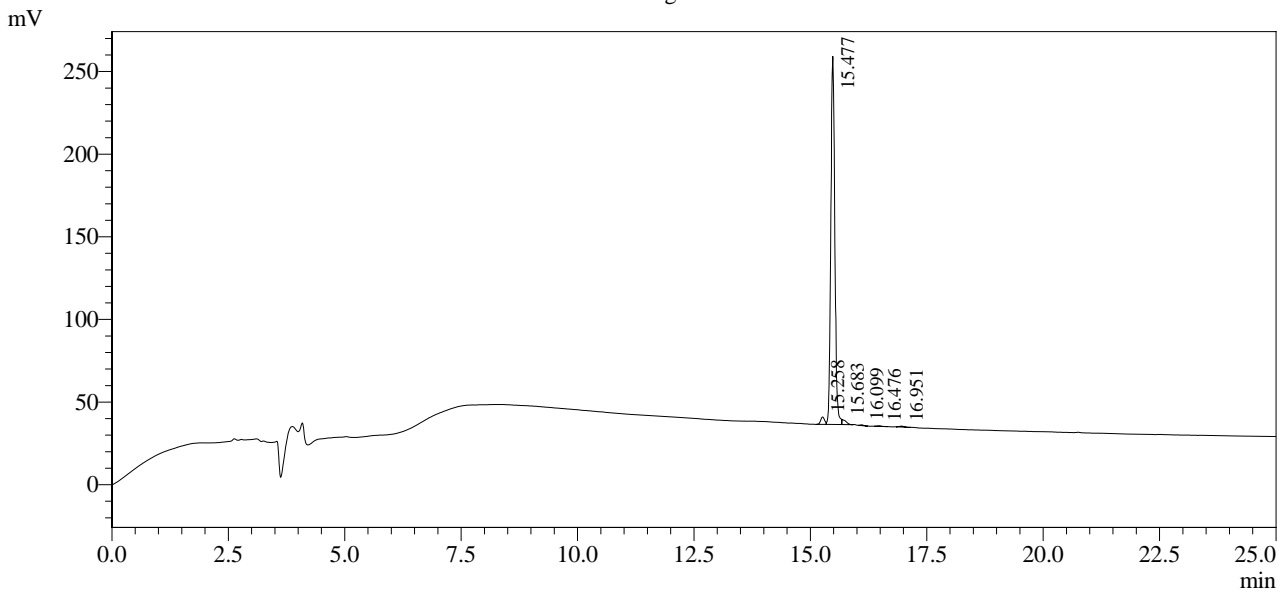

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.258	26614	4493	1.917
2	15.477	1334839	222665	96.154
3	15.683	17946	2955	1.293
4	16.099	2363	481	0.170
5	16.476	2581	360	0.186
6	16.951	3887	552	0.280
Total		1388230	231507	100.000