

Sample Name :LCMV gp33-41  
 Cat. No. : RP20257  
 Lot. No. : E3648119I  
 Time Processed :9:28:05  
 Month-Day-Year Processed :09/09/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GR11010440

Chromatogram

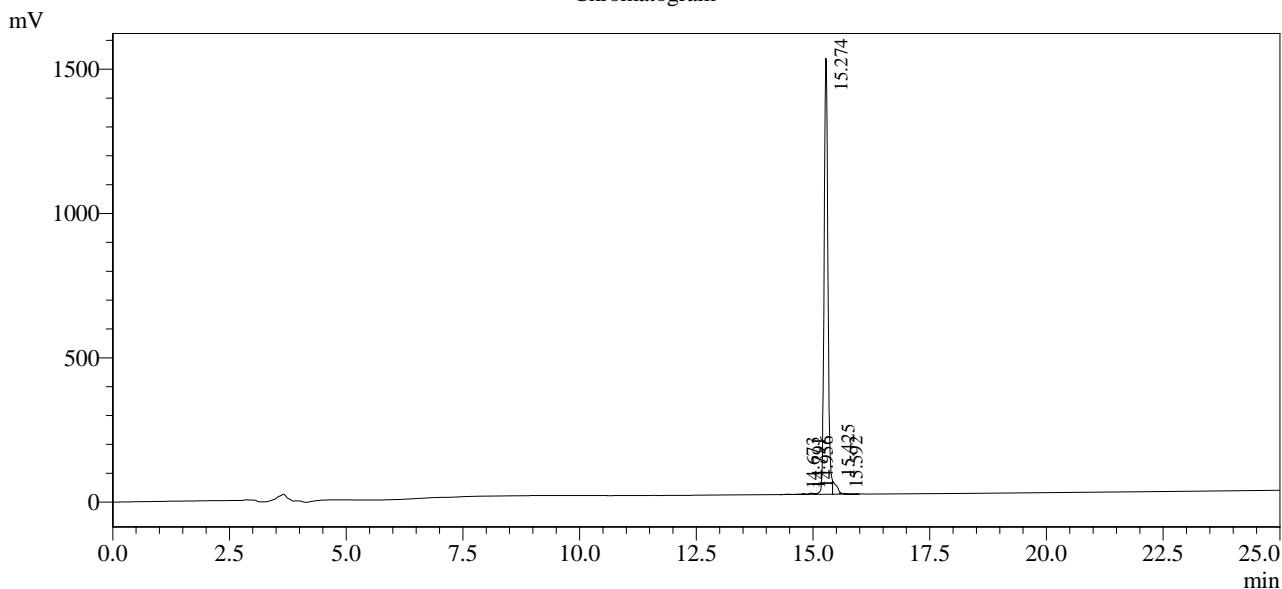

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.673	9438	918	0.106
2	14.791	15732	2552	0.177
3	14.956	30124	4277	0.340
4	15.274	8530517	1510809	96.192
5	15.425	265066	44487	2.989
6	15.592	17378	4365	0.196
Total		8868254	1567407	100.000