

Sample Name :Substance P
 Cat.No :RP10178
 Lot.No : E0433420D
 Time Processed: 13:30:21
 Year-Month-Day: 2020/4/21

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min

<<Detector A>>
 Wavelength Ch1 : 220 nm

<<LC Time Program>>


Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	5	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
27.00	Pumps	Solvent B Conc.	95	
27.01	Pumps	Solvent B Conc.	5	
33.00	Pumps	Solvent B Conc.	5	
33.01	Controller	Stop		

<<Column Performance>>

<Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010015

<Chromatogram>

mV

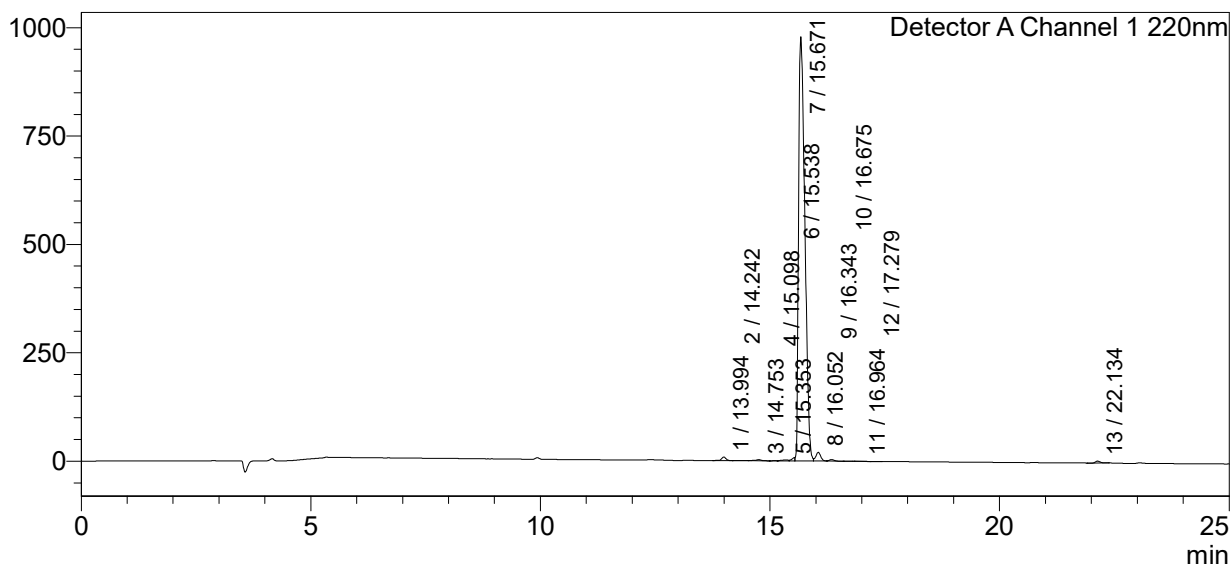

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.994	56157	8263	0.580
2	14.242	1382	90	0.014
3	14.753	24379	2685	0.252
4	15.098	2156	374	0.022
5	15.353	22260	2157	0.230
6	15.538	34136	7636	0.353
7	15.671	9332204	978319	96.409
8	16.052	145558	20033	1.504
9	16.343	23600	3412	0.244
10	16.675	1682	307	0.017
11	16.964	4899	562	0.051
12	17.279	1413	196	0.015
13	22.134	30015	4438	0.310
Total		9679842	1028472	100.000