

Sample Name : OVA Peptide (257-264)  
 Cat. No. : RP10611  
 Lot. No. : E8030421A  
 Time Processed : 16:17:23  
 Month-Day-Year Processed : 01/07/2021  
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment : SS-CM-0310

<Chromatogram>

mV

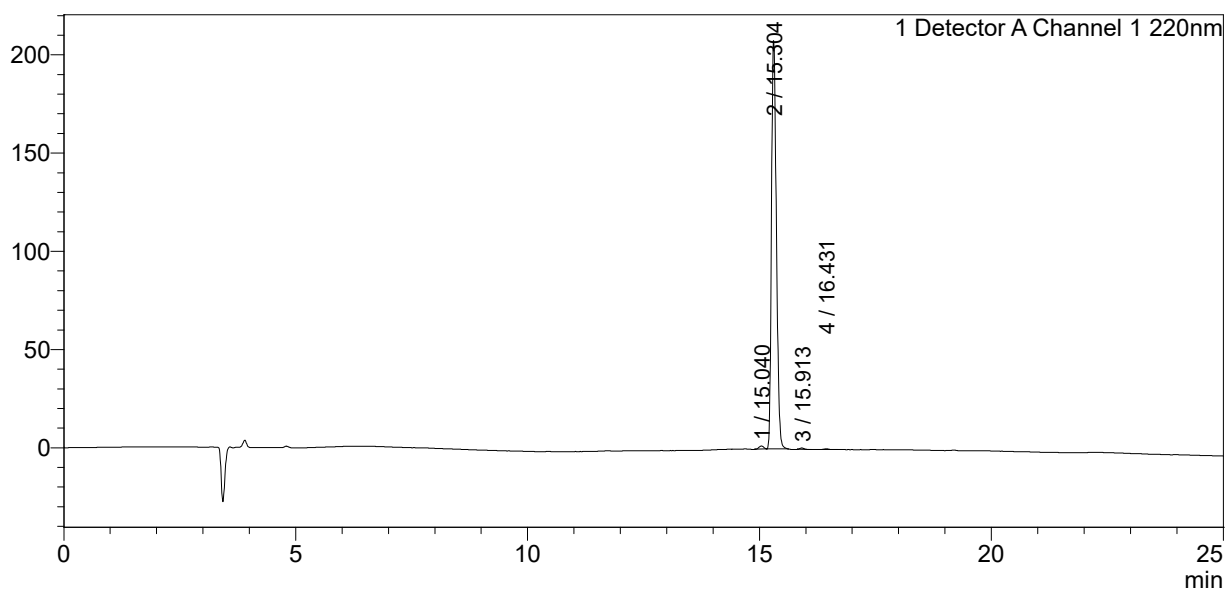

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.040	10679	1547	0.689
2	15.304	1532834	207881	98.919
3	15.913	4401	690	0.284
4	16.431	1666	309	0.108
Total		1549580	210426	100.000