

Sample Name :Exendin-4
 Cat No. :RP10874
 Lot No. :PE8991811
 Time Processed :14:44:03
 Month-Day-Year Processed :11/14/18

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
32.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.00	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

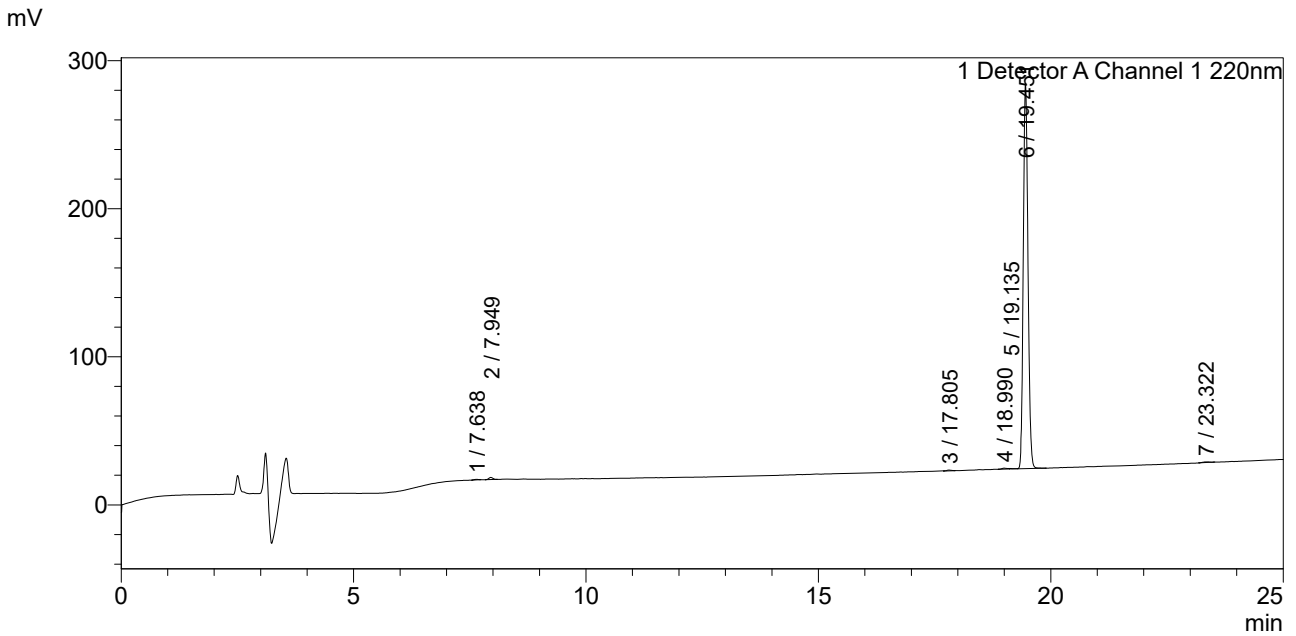

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.638	2212	355	0.120
2	7.949	9077	1465	0.492
3	17.805	3220	501	0.175
4	18.990	5322	637	0.289
5	19.135	2094	297	0.114
6	19.451	1818330	260085	98.591
7	23.322	4065	433	0.220
Total		1844319	263774	100.000