

Sample Name :PACAP (1-38), human, ovine, rat
 Cat. No. : RP10335
 Lot. No. : PE9931806

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

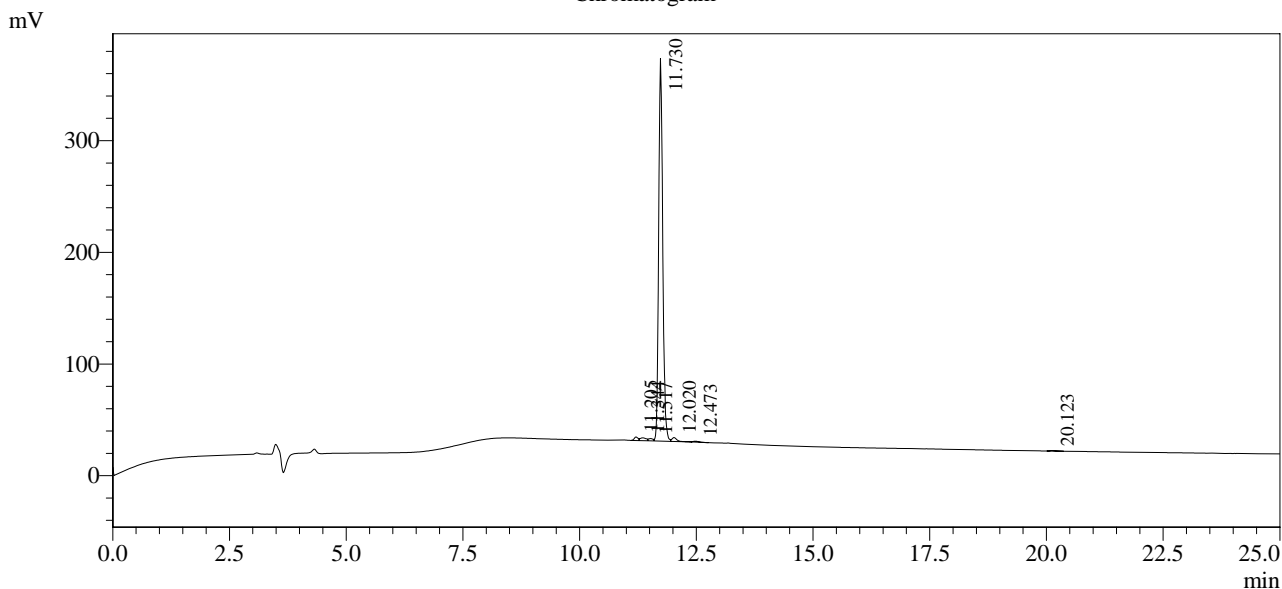

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.205	18423	3191	0.847
2	11.344	23048	2556	1.060
3	11.517	14137	2040	0.650
4	11.730	2085091	342602	95.884
5	12.020	24308	3455	1.118
6	12.473	6198	763	0.285
7	20.123	3386	490	0.156
Total		2174591	355097	100.000