

Sample Name :OVA Peptide (323-339)
 Cat No. :RP10610
 Lot No. :E0743120H
 Time Processed: 5:07:37 AM
 Month-Day-Year Processed :8/28/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010325

<Chromatogram>

mV

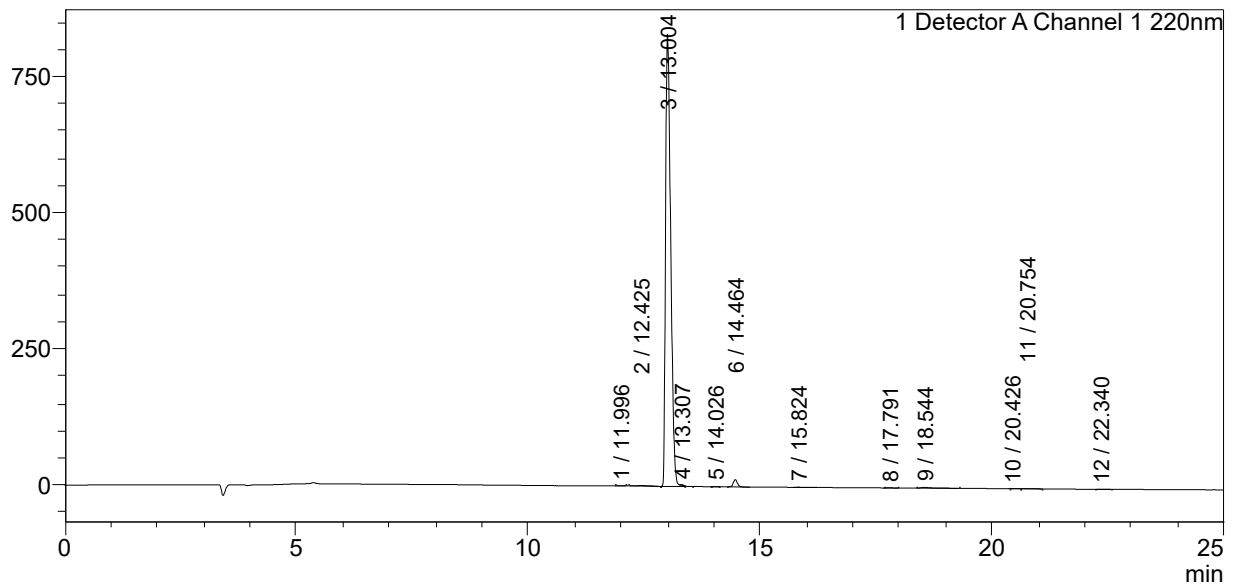

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.996	1868	314	0.029
2	12.425	20452	1001	0.314
3	13.004	6376803	830441	97.774
4	13.307	4687	1216	0.072
5	14.026	1492	293	0.023
6	14.464	83557	13433	1.281
7	15.824	2470	230	0.038
8	17.791	1249	141	0.019
9	18.544	23875	1583	0.366
10	20.426	1208	172	0.019
11	20.754	2994	275	0.046
12	22.340	1346	181	0.021
Total		6522000	849280	100.000