

Sample Name : Substance P  
 Cat. No. : RP10178  
 Lot. No. : PE5821904  
 Time Processed :8:56:52  
 Month-Day-Year Processed :04/17/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GR11010440

Chromatogram

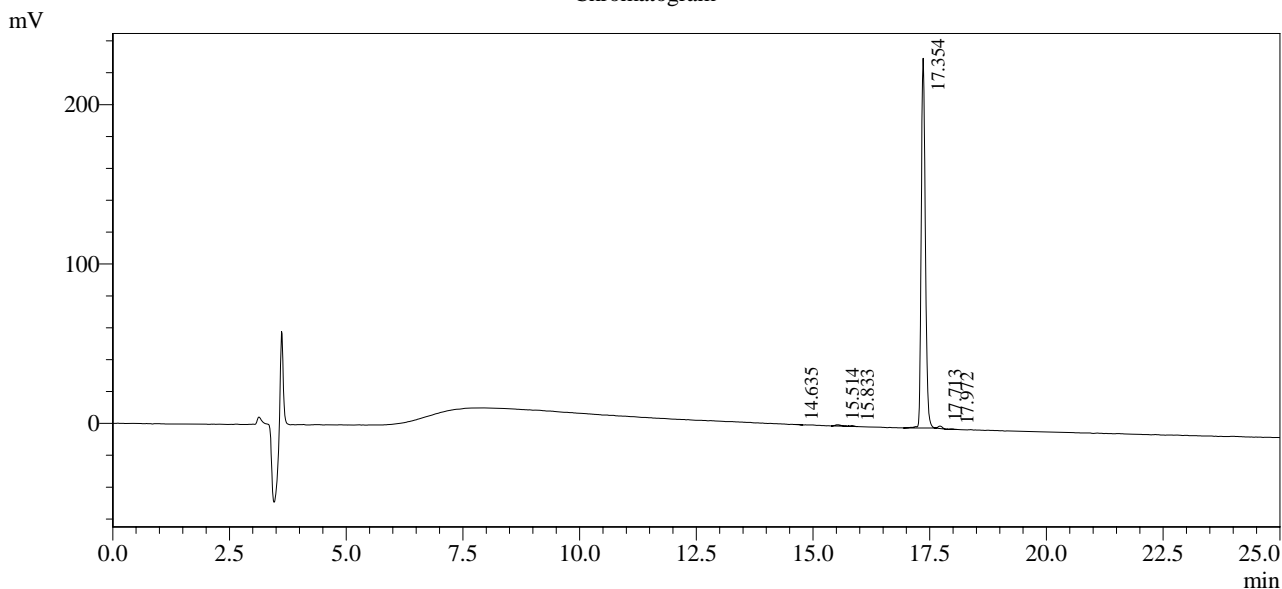

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.635	1180	156	0.082
2	15.514	7913	840	0.546
3	15.833	2478	495	0.171
4	17.354	1424748	232019	98.402
5	17.713	9882	1519	0.682
6	17.972	1682	273	0.116
Total		1447882	235301	100.000