

Sample Name : CEF20
 Cat No.: RP11781
 Lot No.: E2088120F
 Time Processed : 9:23:19
 Month-Day-Year Processed : 07/02/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010014

<Chromatogram>

mV

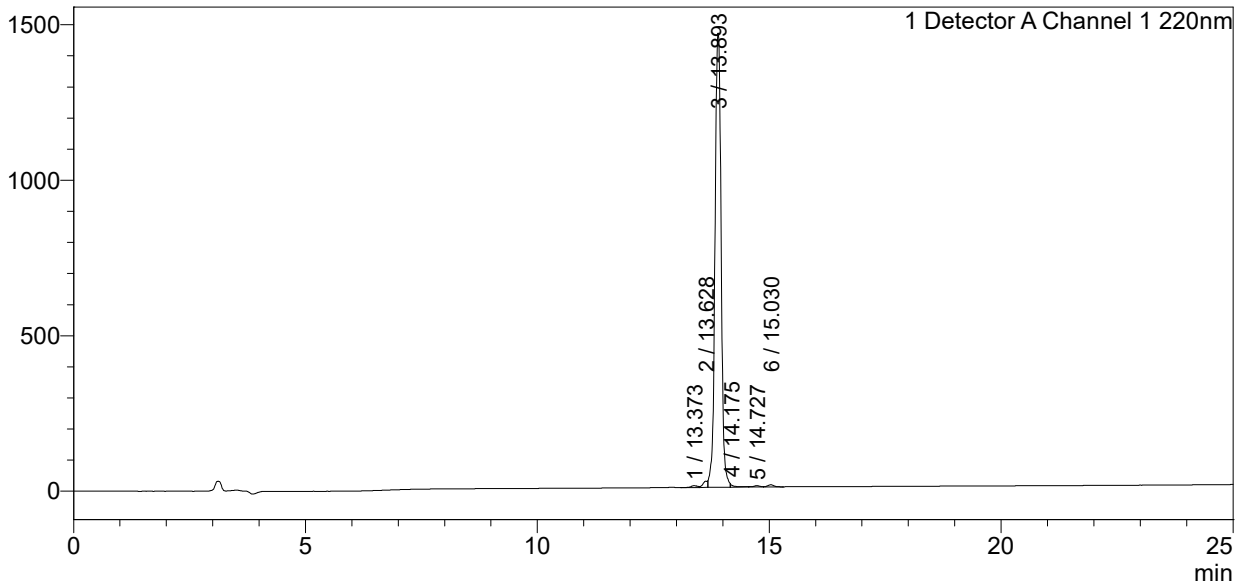

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.373	56381	5870	0.410
2	13.628	140908	19675	1.025
3	13.893	13381405	1453576	97.386
4	14.175	57511	9054	0.419
5	14.727	41350	4329	0.301
6	15.030	63021	6793	0.459
Total		13740575	1499297	100.000