

Sample Name: CEF20
 Cat No. : RP11781
 Lot No. : E7938120H
 Time Processed: 9:44:18
 Month-Day-Year Processed :09/03/2020
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010014

<Chromatogram>

mV

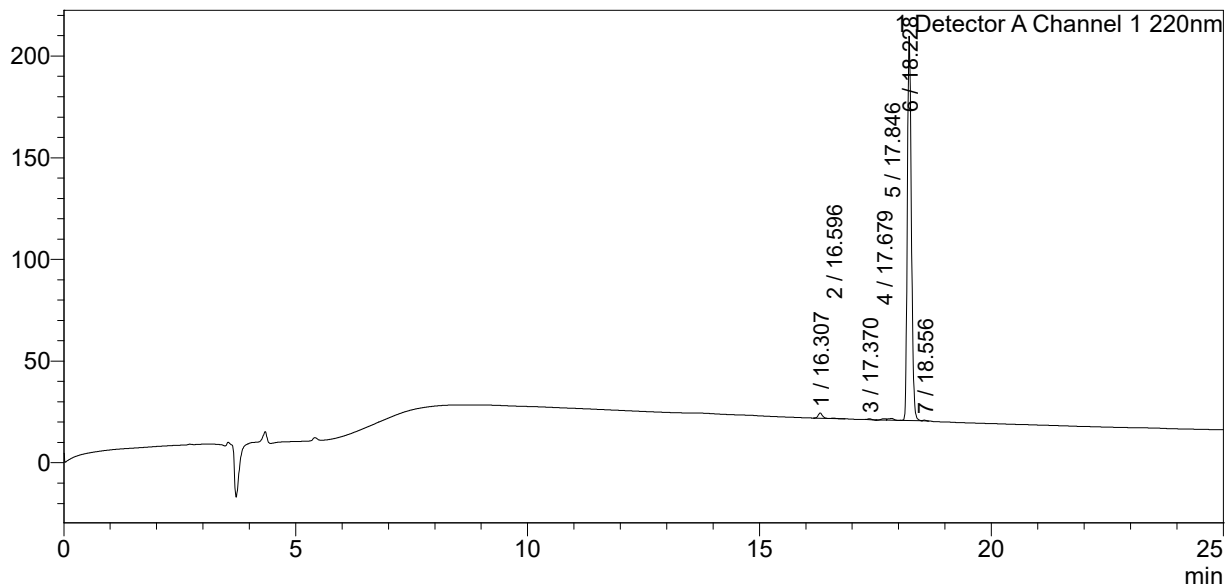

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.307	16385	2574	1.393
2	16.596	1734	292	0.147
3	17.370	2549	472	0.217
4	17.679	5254	691	0.447
5	17.846	7651	882	0.650
6	18.228	1141386	189040	97.037
7	18.556	1284	320	0.109
Total		1176244	194271	100.000