


# Mass Spectrum

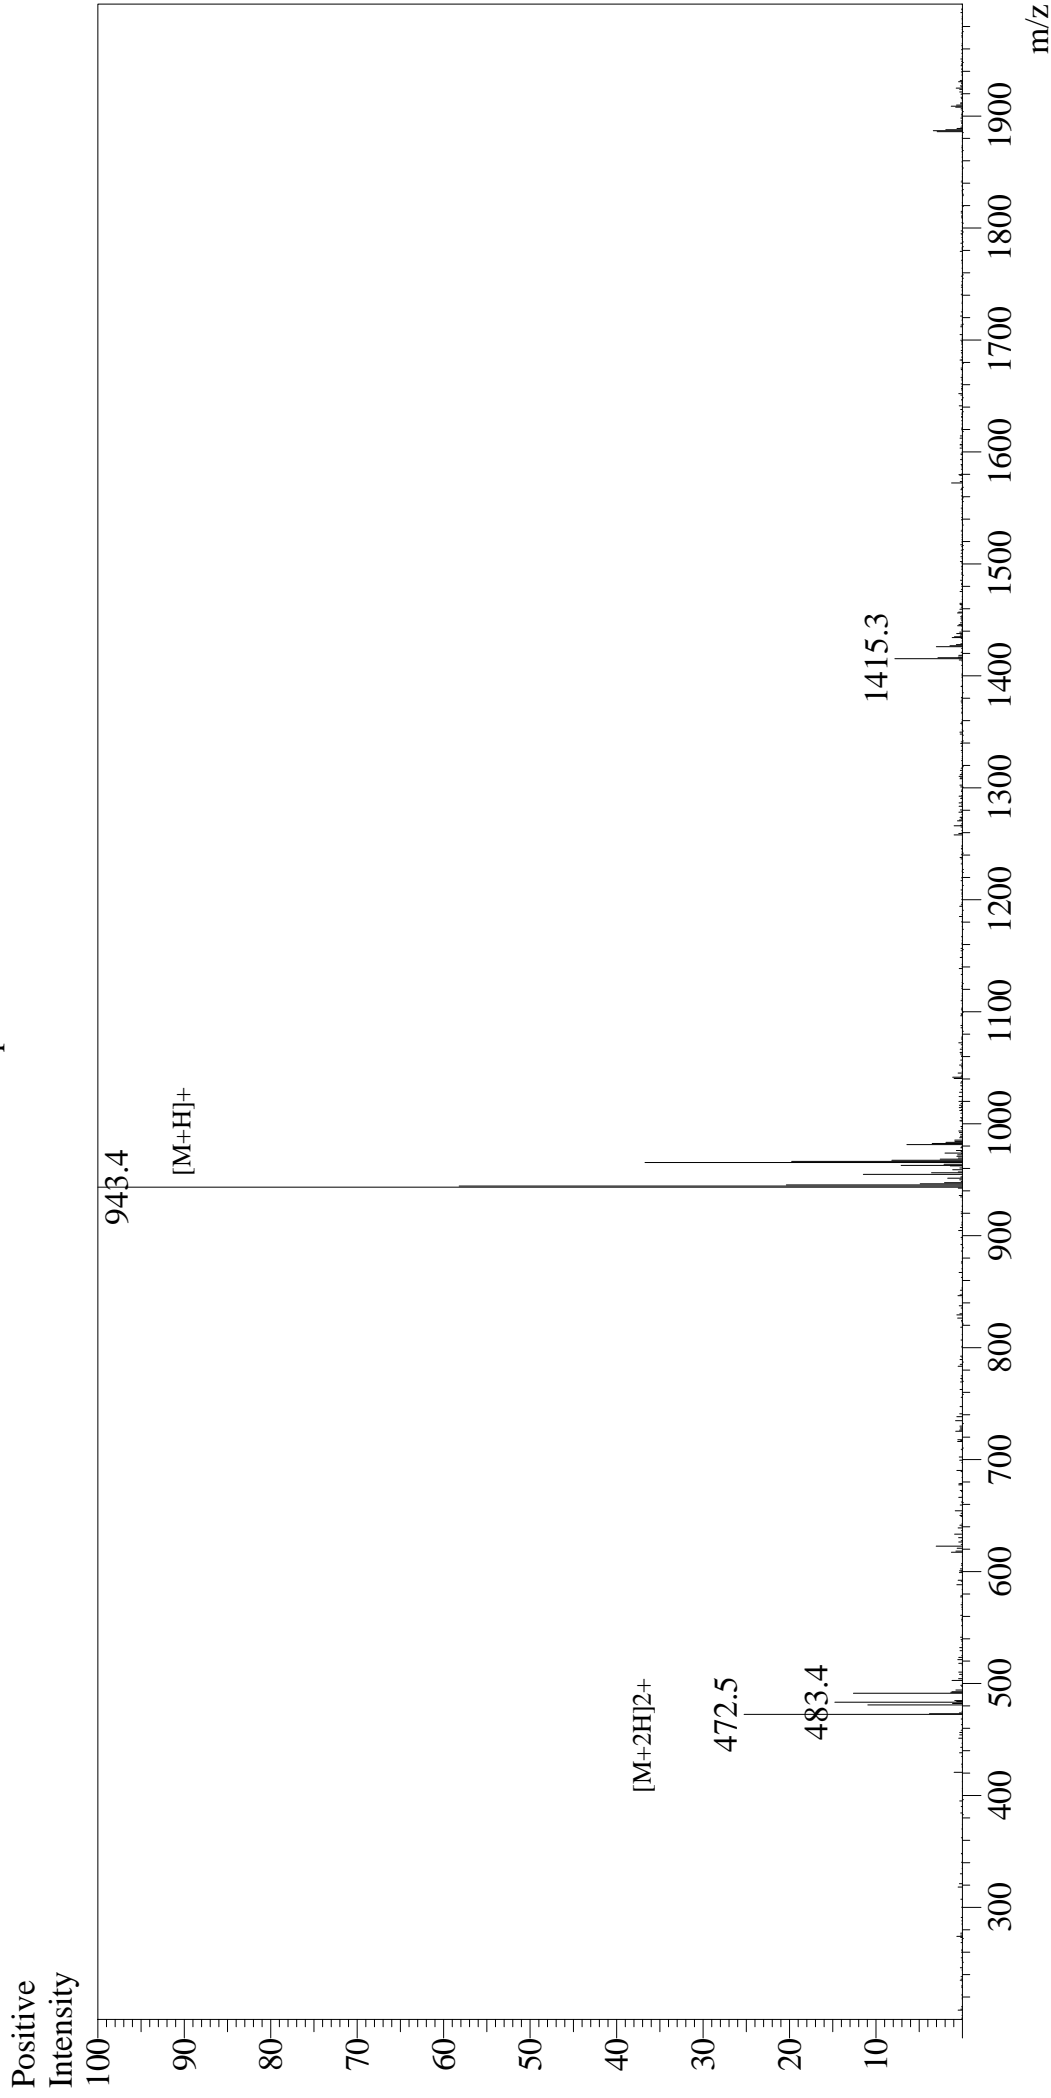

## Sample Information

Month-Day Processed : 09/02/20  
Time Processed : 22:56:10  
Injection Volume : 0.3  
Sample Name : CEF20  
Cat No. : RP11781  
Lot No. : E7938120H  
Theoretical MW : 943.18  
Observed MW : 942.4

Interface : ESI  
Nebulizing Gas Flow : 1.5L/min  
CDL Temp : 250  
Block Temp : 200

Equipment : GK11010007  
Interface Bias : +4.5kV  
Drying Gas Flow : 5 L/min  
T.Flow : 0.2ml/min  
B.conc : 50%H2O/50%MeOH