

Sample Name :RGD  
 Cat No. :RP20297  
 Lot No. :E1580021G  
 Time Processed :12:47:50  
 Month-Day-Year Processed :07/17/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm  
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

<Chromatogram>

mV

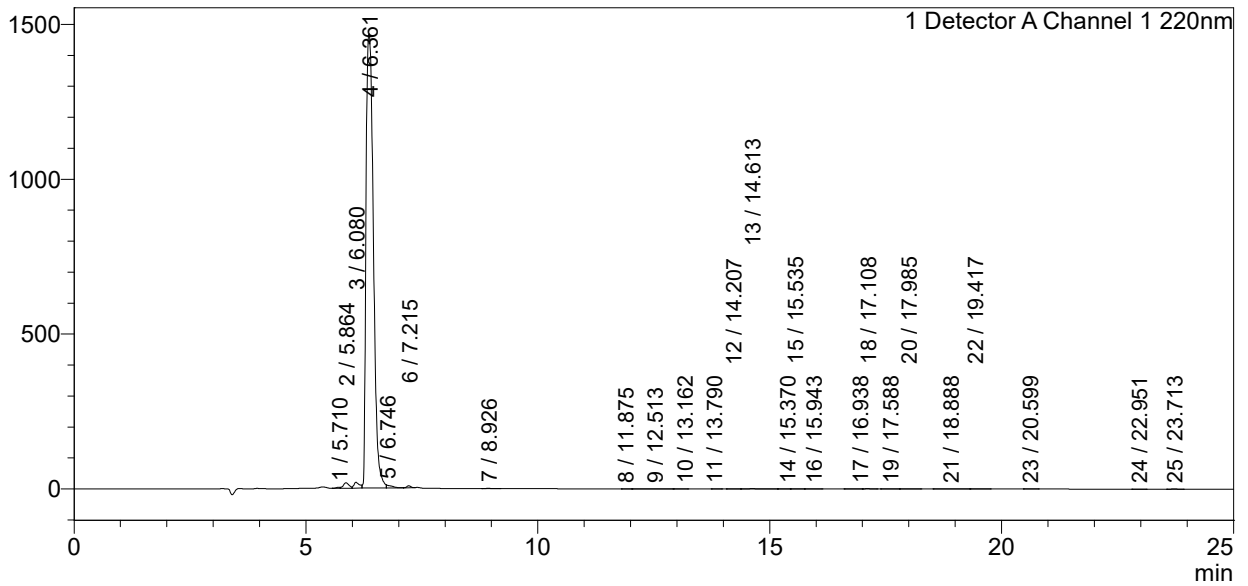

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.710	18729	3282	0.113
2	5.864	149193	17708	0.899
3	6.080	161082	18934	0.970
4	6.361	16061785	1467625	96.763
5	6.746	78086	9419	0.470
6	7.215	39135	6466	0.236
7	8.926	6911	928	0.042
8	11.875	1091	77	0.007
9	12.513	13554	451	0.082
10	13.162	1450	127	0.009
11	13.790	1403	129	0.008
12	14.207	2178	195	0.013
13	14.613	10740	762	0.065
14	15.370	1920	189	0.012

Peak#	Ret. Time	Area	Height	Area%
15	15.535	3166	248	0.019
16	15.943	2434	153	0.015
17	16.938	4579	329	0.028
18	17.108	8205	756	0.049
19	17.588	3829	245	0.023
20	17.985	1399	96	0.008
21	18.888	18176	621	0.110
22	19.417	4811	282	0.029
23	20.599	1499	164	0.009
24	22.951	1198	92	0.007
25	23.713	2596	264	0.016
Total		16599149	1529542	100.000