

Sample Name : PACAP (1-38), human, ovine, rat
 Cat No. : RP10335
 Lot No. : E7720520A
 Time Processed : 0:36:54
 Month-Day-Year Processed : 02/07/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK12010012

<Chromatogram>

mV

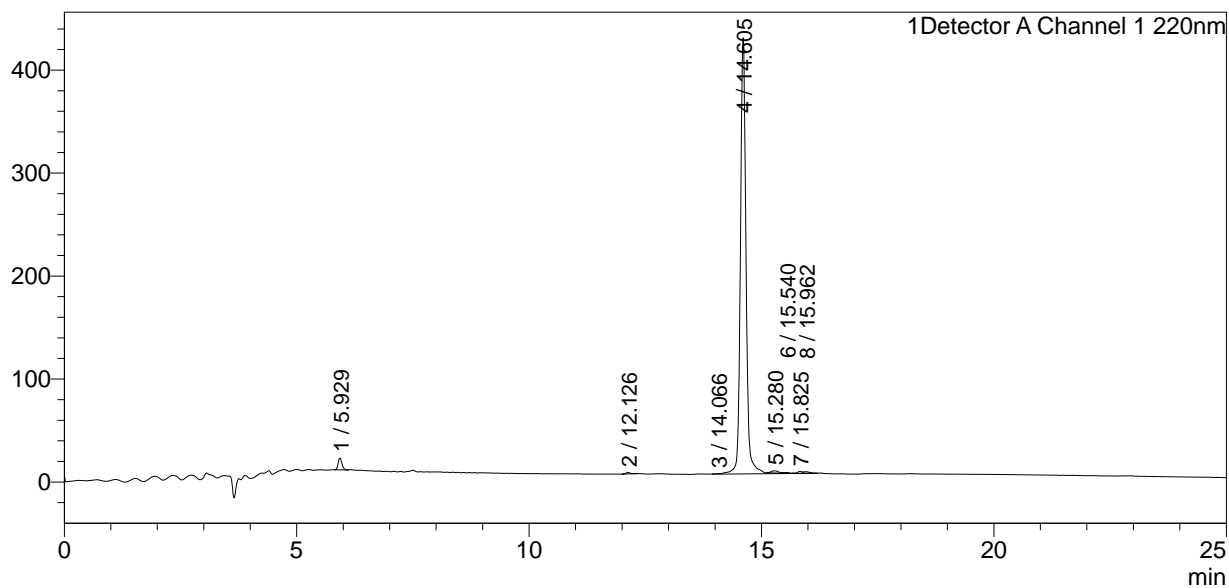

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.929	63955	11402	1.740
2	12.126	9687	1444	0.263
3	14.066	3038	467	0.083
4	14.605	3544898	423441	96.421
5	15.280	23373	2118	0.636
6	15.540	4914	710	0.134
7	15.825	12717	1762	0.346
8	15.962	13897	1506	0.378
Total		3676478	442849	100.000