

Sample Name :HA Peptide  
 Cat No. :RP11735  
 Lot No. :E1986120E  
 Time Processed :11:09:43  
 Month-Day-Year Processed :05/30/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm  
 Equipment:ZJ19010141

<Chromatogram>

mV

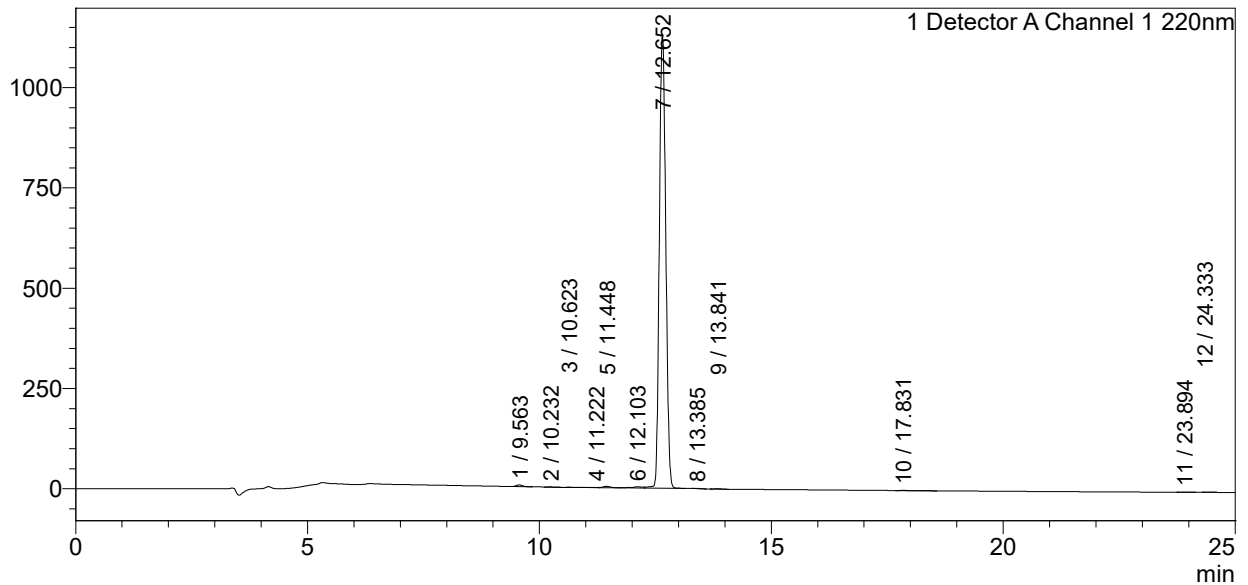

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.563	36786	4026	0.334
2	10.232	4368	457	0.040
3	10.623	2888	355	0.026
4	11.222	5413	486	0.049
5	11.448	34929	3412	0.317
6	12.103	48136	2719	0.436
7	12.652	10874634	1132390	98.598
8	13.385	3383	389	0.031
9	13.841	8794	869	0.080
10	17.831	7171	386	0.065
11	23.894	1668	133	0.015
12	24.333	1052	116	0.010
Total		11029222	1145737	100.000