

Sample Name: Calcitonin Gene Related Peptide (CGRP) (8-37), rat
 Cat No : RP11090
 Lot No : E1975821E
 Time Processed : 7:45:09 PM
 Month-Day-Year Processed : 05/13/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: SS-CM-0309

<Chromatogram>

mV

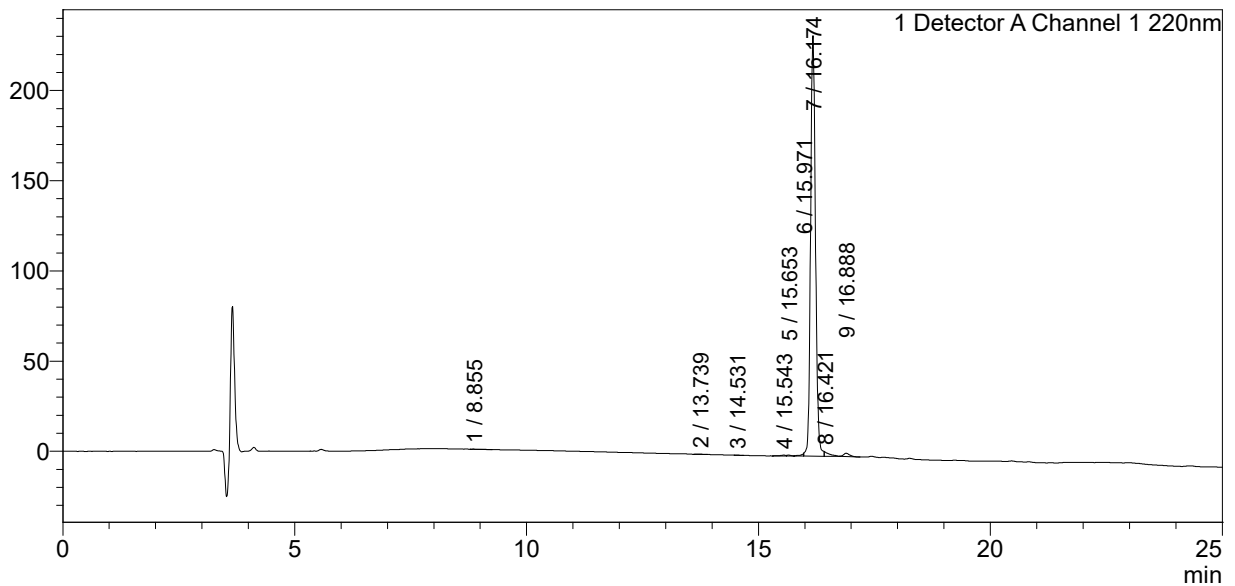

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.855	2438	145	0.138
2	13.739	1802	243	0.102
3	14.531	1042	195	0.059
4	15.543	4668	476	0.264
5	15.653	3209	514	0.181
6	15.971	6831	1388	0.386
7	16.174	1714184	233162	96.910
8	16.421	18192	2592	1.028
9	16.888	16482	1827	0.932
Total		1768848	240542	100.000