

Sample Name :Neuropeptide Y, human
 Cat No.: RP10492
 Lot No.:E92028201
 Time Processed :17:16:27
 Month-Day-Year Processed :10/08/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	0
25.00	Pumps	Pump A B.Conc	60
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	0
40.00	Pumps	Pump A B.Conc	0
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010014

<Chromatogram>

mV

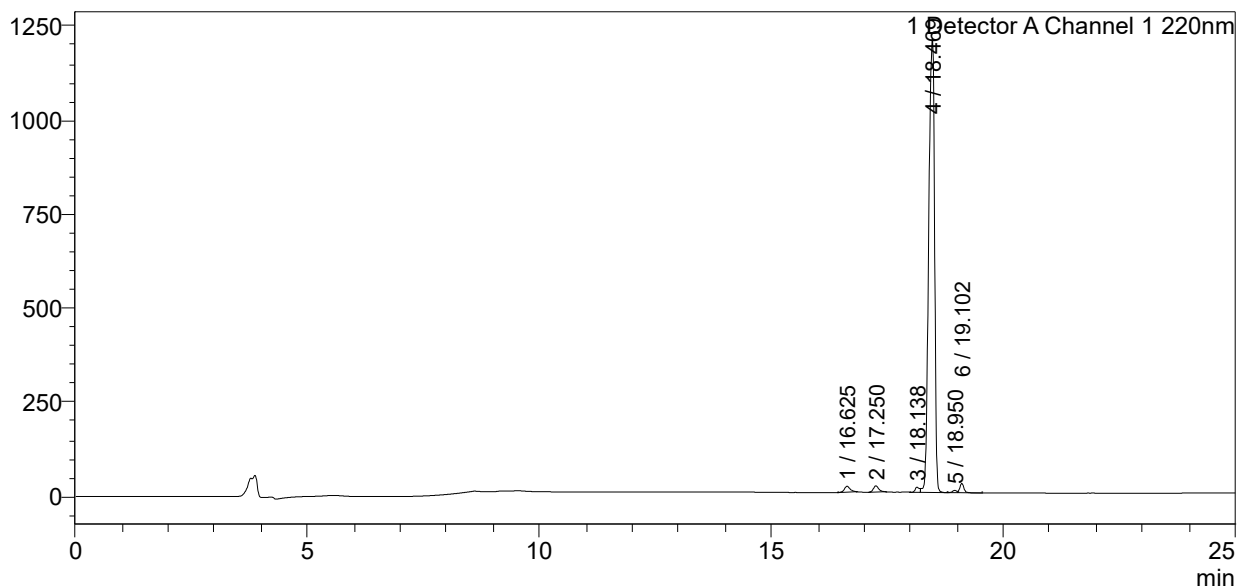

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.625	142715	15988	1.292
2	17.250	135027	16796	1.222
3	18.138	78608	13870	0.711
4	18.469	10498610	1208657	95.023
5	18.950	40713	6287	0.368
6	19.102	152860	25310	1.384
Total		11048533	1286908	100.000