

Sample Name :OVA Peptide (323-339)  
 Cat No. :RP10610  
 Lot No. :E6863120A  
 Time Processed :7:43:43  
 Month-Day-Year Processed :01/22/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ17010507

<Chromatogram>

mV

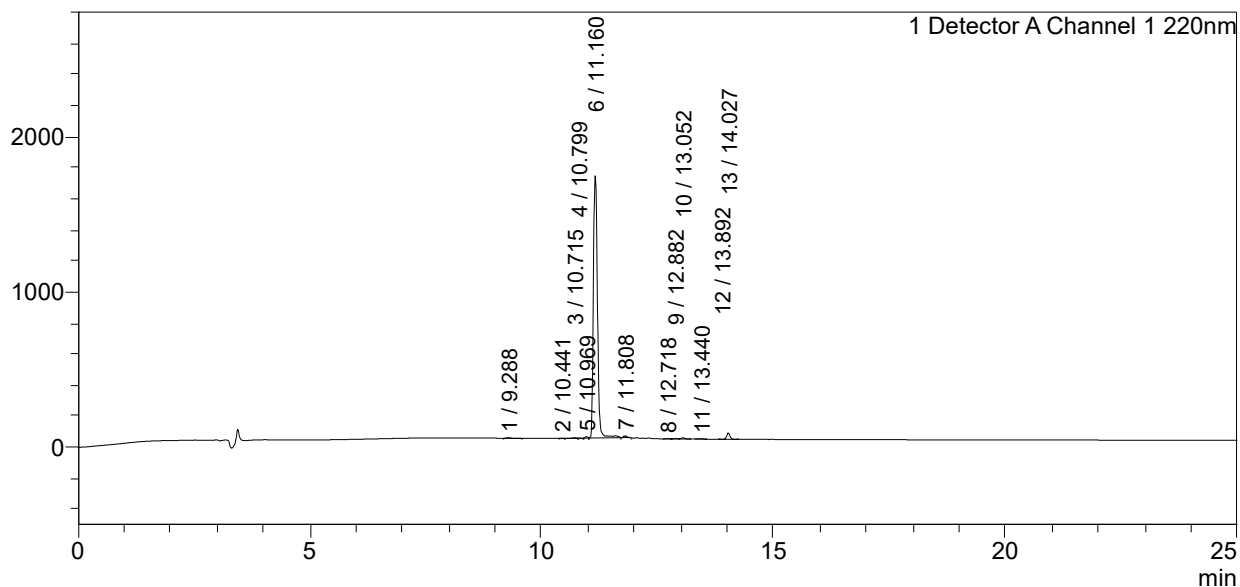

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.288	20424	3850	0.189
2	10.441	1535	444	0.014
3	10.715	31855	4224	0.295
4	10.799	11888	2931	0.110
5	10.969	52850	10209	0.490
6	11.160	10346391	1688350	95.922
7	11.808	47917	10691	0.444
8	12.718	6978	1498	0.065
9	12.882	9180	1540	0.085
10	13.052	37526	7507	0.348
11	13.440	19224	3786	0.178
12	13.892	1314	324	0.012
13	14.027	199142	40336	1.846
Total		10786224	1775692	100.000