

Sample Name : Melittin,honey bee
 Cat. No. : RP20415
 Lot. No. : E8080621C
 Time Processed :9:18:36
 Month-Day-Year Processed :03/11/2021
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ20010140

<Chromatogram>

mV

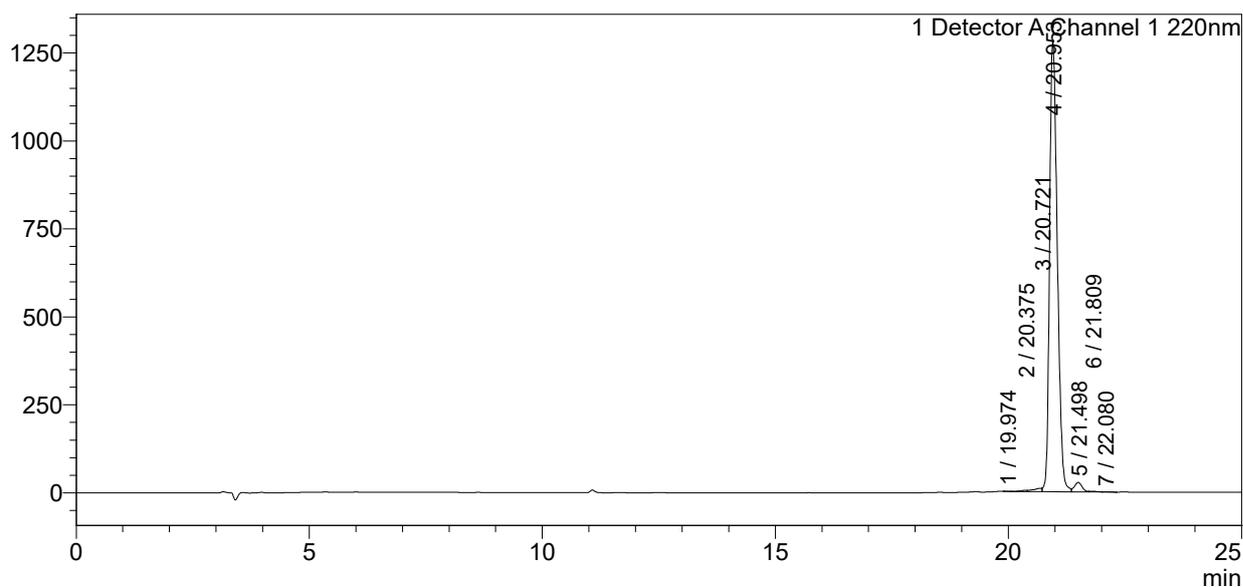

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	19.974	1792	305	0.012
2	20.375	39749	3587	0.261
3	20.721	127068	10163	0.835
4	20.953	14716024	1283850	96.671
5	21.498	308671	26957	2.028
6	21.809	22378	2075	0.147
7	22.080	7116	698	0.047
Total		15222798	1327634	100.000