

Sample Name :RGD  
 Cat No. :RP20297  
 Lot No. :E9409920B  
 Time Processed :9:15:05  
 Month-Day-Year Processed :02/21/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>  
 Column : Alltima™ C18 4.6 x 250 mm  
 Equipment:ZJ19010141

<Chromatogram>

mV

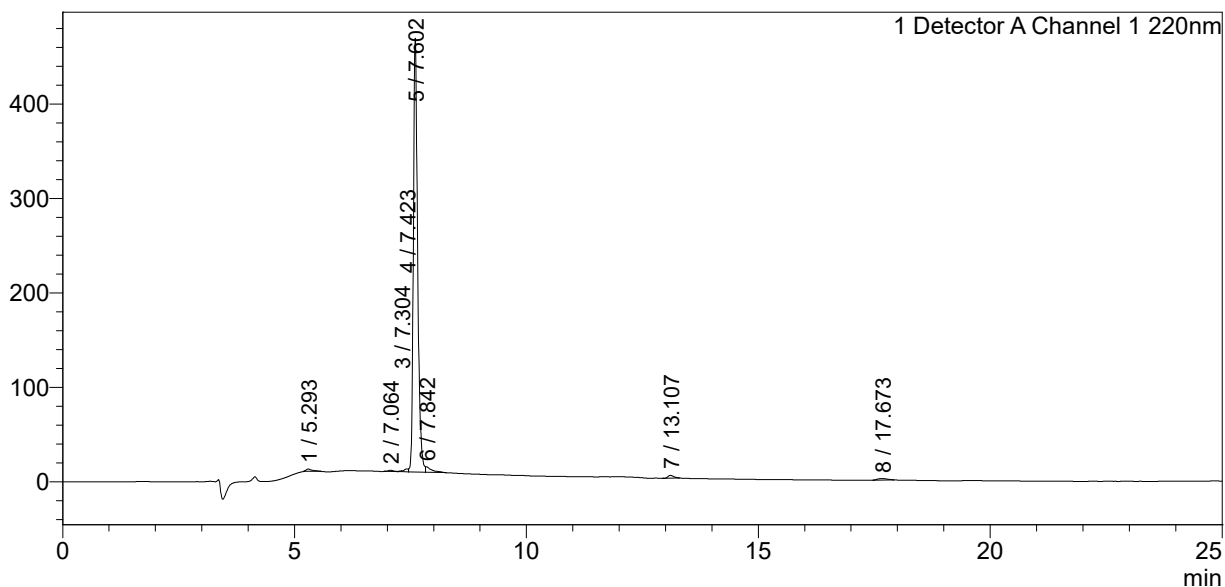

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.293	21889	2378	0.700
2	7.064	9672	1236	0.309
3	7.304	3039	851	0.097
4	7.423	20071	3069	0.642
5	7.602	2972671	459551	95.032
6	7.842	52655	5807	1.683
7	13.107	25863	3006	0.827
8	17.673	22213	1528	0.710
Total		3128074	477425	100.000