

Sample Name :Melittin,honey bee
 Cat No. : RP20415
 Lot No. : E8228521C
 Time Processed :6:45:47
 Month-Day-Year Processed :03/13/2021
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: SS-CM-0310

<Chromatogram>

mV

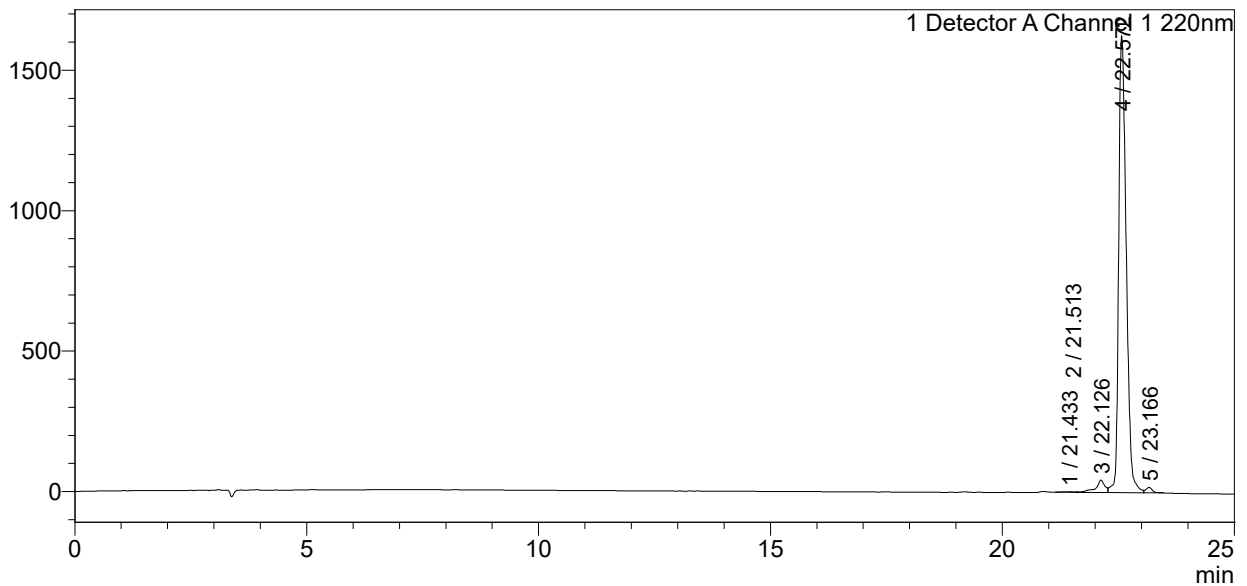

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	21.433	23710	1978	0.123
2	21.513	17012	2072	0.089
3	22.126	602885	44177	3.140
4	22.572	18378097	1627319	95.711
5	23.166	179905	19153	0.937
Total		19201608	1694699	100.000