

Sample Name: Gastric Inhibitory Peptide (GIP), human  
 Cat No. :RP10795  
 Lot No. :E6152520J  
 Time Processed: 8:46:36 AM  
 Month-Day-Year Processed :11/10/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm  
 Equipment: ZJ19010325

<Chromatogram>

mV

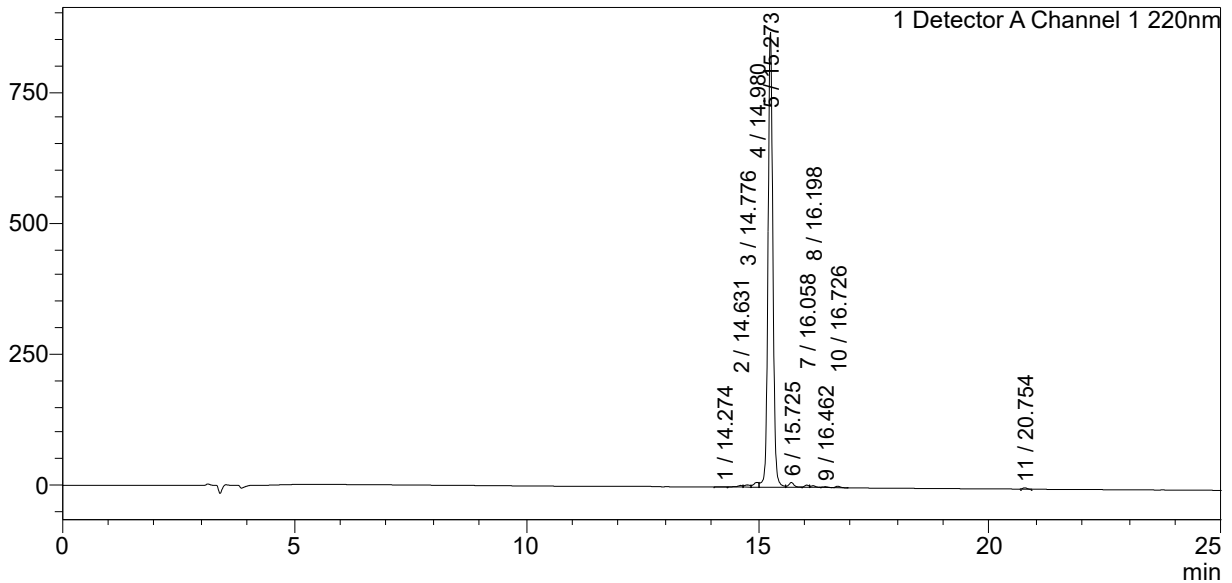

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.274	3862	418	0.059
2	14.631	27817	3063	0.423
3	14.776	34785	4278	0.528
4	14.980	74475	8893	1.131
5	15.273	6283638	865914	95.446
6	15.725	68164	9127	1.035
7	16.058	28601	4045	0.434
8	16.198	16345	2827	0.248
9	16.462	10194	1262	0.155
10	16.726	20110	2827	0.305
11	20.754	15459	2528	0.235
Total		6583449	905180	100.000