

Sample Name : Rabies Virus Glycoprotein
 Cat. No. : RP20464
 Lot. No. : E4266220H
 Time Processed : 9:00:50
 Month-Day-Year Processed : 08/16/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

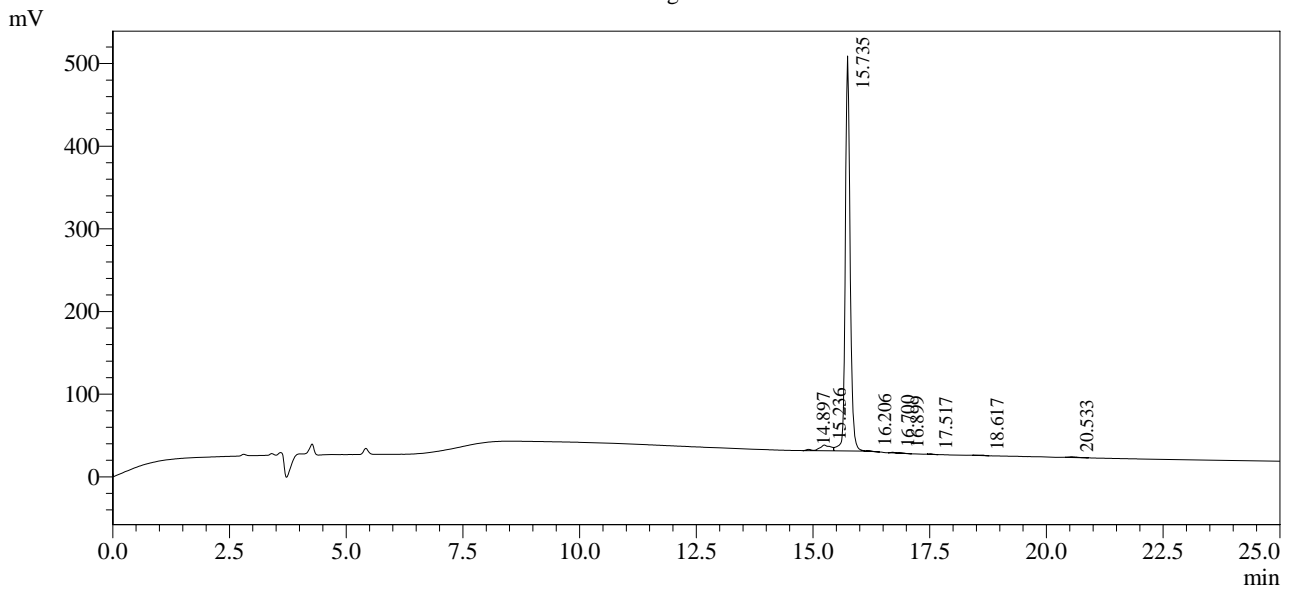

1 Det.A Ch1 / 220nm
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.897	11333	1522	0.315
2	15.236	107814	6920	2.996
3	15.735	3447472	477919	95.787
4	16.206	5019	804	0.139
5	16.700	4565	824	0.127
6	16.899	2380	396	0.066
7	17.517	3342	557	0.093
8	18.617	6093	607	0.169
9	20.533	11092	916	0.308
Total		3599109	490465	100.000