

Sample Name :Hexa-His  
 Cat No. :RP11737  
 Lot No. :E9494921H  
 Time Processed : 16:36:19  
 Month-Day-Year Processed : 08/05/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
32.00	Pumps	B.Conc	95
32.01	Pumps	B.Conc	5
45.00	Pumps	B.Conc	5
45.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010017

mV

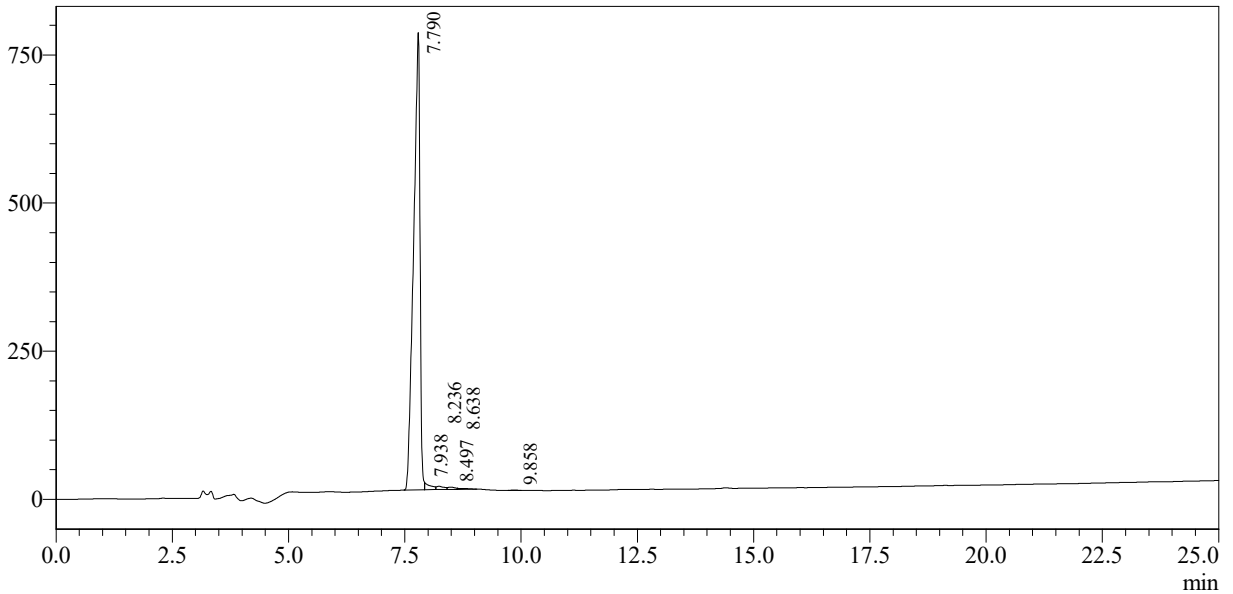

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	7.790	7328889	771406	96.908
2	7.938	101259	11443	1.339
3	8.236	64133	5661	0.848
4	8.497	41278	3868	0.546
5	8.638	23421	1784	0.310
6	9.858	3757	486	0.050
Total		7562738	794647	100.000