

Sample Name: Calcitonin Gene Related Peptide (CGRP), rat
 Cat No : RP11095
 Lot No : E9406121D
 Time Processed : 8:13:08
 Month-Day-Year Processed : 04/30/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010011

<Chromatogram>

mV

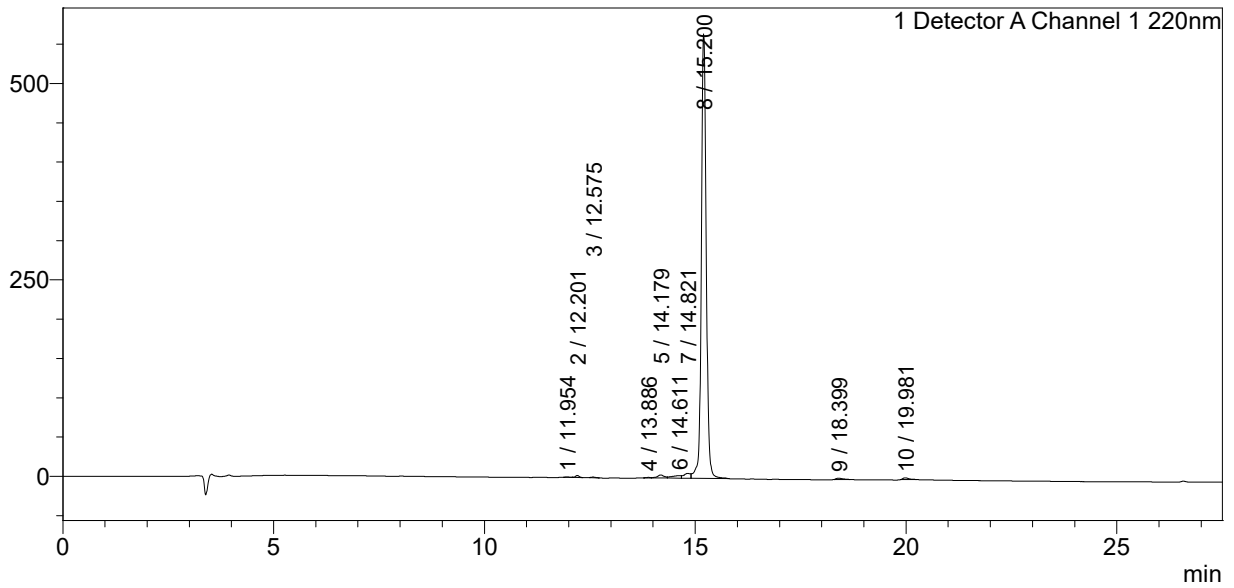

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.954	3418	577	0.071
2	12.201	14694	2478	0.306
3	12.575	4431	695	0.092
4	13.886	4753	606	0.099
5	14.179	45675	3951	0.950
6	14.611	49929	3315	1.038
7	14.821	68434	6237	1.423
8	15.200	4578340	565978	95.195
9	18.399	17514	1713	0.364
10	19.981	22251	2239	0.463
Total		4809439	587789	100.000