

Sample Name : HA Peptide
 Cat. No. : RP11735
 Lot. No. : PE4851611

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


| Time | Unit | Command | Value | Comment |
|-------|------------|--------------|-------|---------|
| 0.01 | Pumps | Pump B Conc. | 5 | |
| 25.00 | Pumps | Pump B Conc. | 65 | |
| 25.01 | Pumps | Pump B Conc. | 95 | |
| 31.00 | Pumps | Pump B Conc. | 95 | |
| 31.01 | Pumps | Pump B Conc. | 5 | |
| 40.00 | Pumps | Pump B Conc. | 5 | |
| 40.01 | Controller | Stop | | |

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

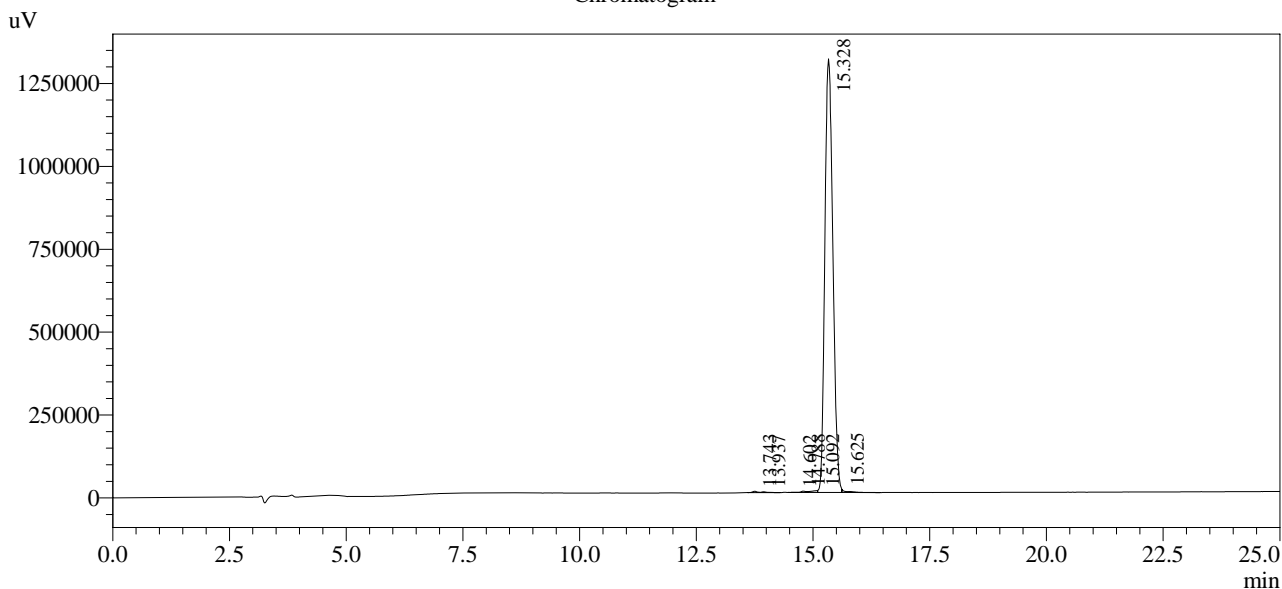

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

| Peak# | Ret. Time | Area | Height | Area % |
|-------|-----------|----------|---------|---------|
| 1 | 13.743 | 29790 | 4104 | 0.188 |
| 2 | 13.937 | 24668 | 2535 | 0.156 |
| 3 | 14.602 | 4363 | 492 | 0.028 |
| 4 | 14.788 | 28385 | 4152 | 0.179 |
| 5 | 15.092 | 58409 | 5981 | 0.369 |
| 6 | 15.328 | 15612902 | 1308148 | 98.646 |
| 7 | 15.625 | 68716 | 8217 | 0.434 |
| Total | | 15827233 | 1333629 | 100.000 |