

Sample Name :PAR-4 Agonist Peptide, amide
 Cat No. :RP11529
 Lot No. :E8185621C
 Time Processed :18:23:37
 Month-Day-Year Processed :03/14/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

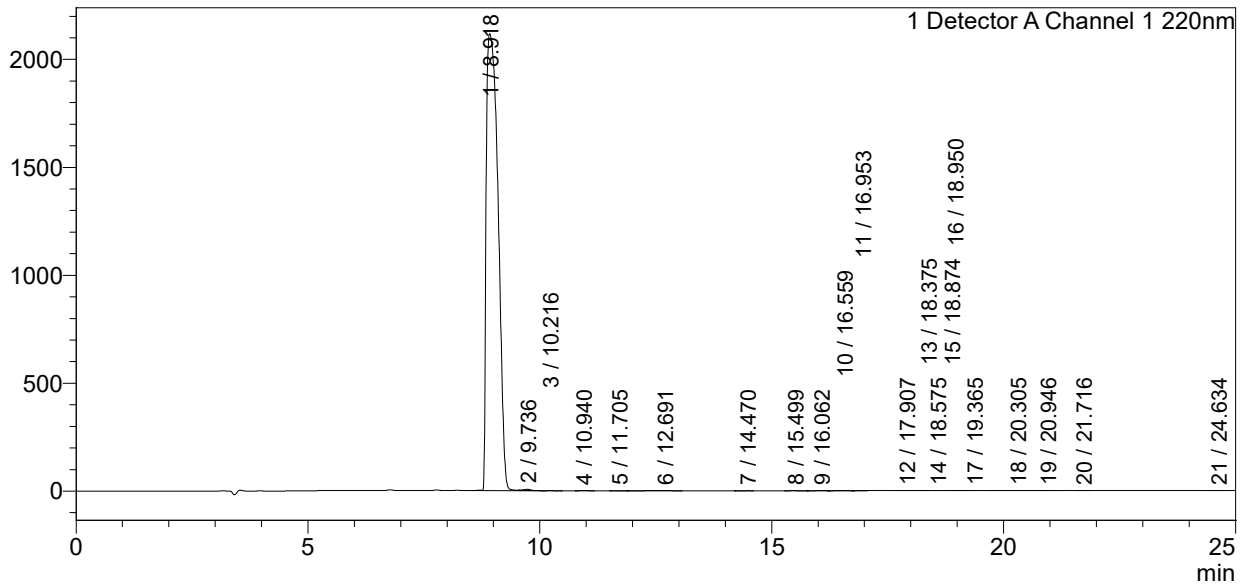

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.918	37315937	2117000	99.602
2	9.736	52054	5268	0.139
3	10.216	2611	291	0.007
4	10.940	11679	1411	0.031
5	11.705	1081	119	0.003
6	12.691	15995	507	0.043
7	14.470	2220	178	0.006
8	15.499	2182	130	0.006
9	16.062	3728	365	0.010
10	16.559	4049	244	0.011
11	16.953	1618	130	0.004
12	17.907	8525	443	0.023
13	18.375	1182	143	0.003
14	18.575	1231	133	0.003

Peak#	Ret. Time	Area	Height	Area%
15	18.874	1269	145	0.003
16	18.950	1023	129	0.003
17	19.365	1019	104	0.003
18	20.305	28922	770	0.077
19	20.946	4846	307	0.013
20	21.716	1759	176	0.005
21	24.634	2218	212	0.006
Total		37465148	2128205	100.000