

Sample Name :Substance P
 Cat No :RP10178
 Lot No :E8445921B
 Time Processed :21:14:26
 Month-Day-Year Processed :02/10/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: SS-CM-0309

<Chromatogram>

mV

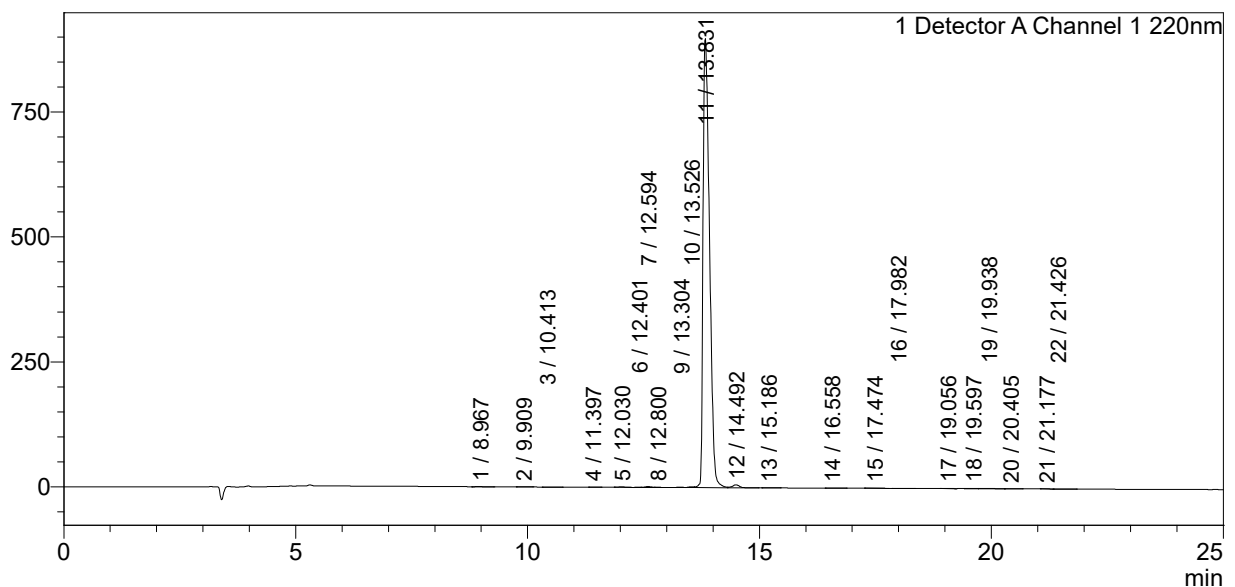

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.967	1535	121	0.017
2	9.909	1094	95	0.012
3	10.413	1636	112	0.019
4	11.397	1260	119	0.014
5	12.030	8600	1097	0.097
6	12.401	1894	295	0.021
7	12.594	15755	1642	0.179
8	12.800	3078	546	0.035
9	13.304	5301	557	0.060
10	13.526	11887	1565	0.135
11	13.831	8675364	898328	98.356
12	14.492	63810	5874	0.723
13	15.186	1019	90	0.012
14	16.558	2178	142	0.025
15	17.474	5486	368	0.062
16	17.982	1517	116	0.017

Peak#	Ret. Time	Area	Height	Area%
17	19.056	1618	164	0.018
18	19.597	4977	332	0.056
19	19.938	8342	400	0.095
20	20.405	1519	126	0.017
21	21.177	1366	195	0.015
22	21.426	1091	66	0.012
Total		8820328	912351	100.000