

Sample Name :PAR-4 Agonist Peptide, amide
 Cat No. :RP11529
 Lot No. :E4122821H
 Time Processed :10:11:35
 Month-Day-Year Processed :08/11/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

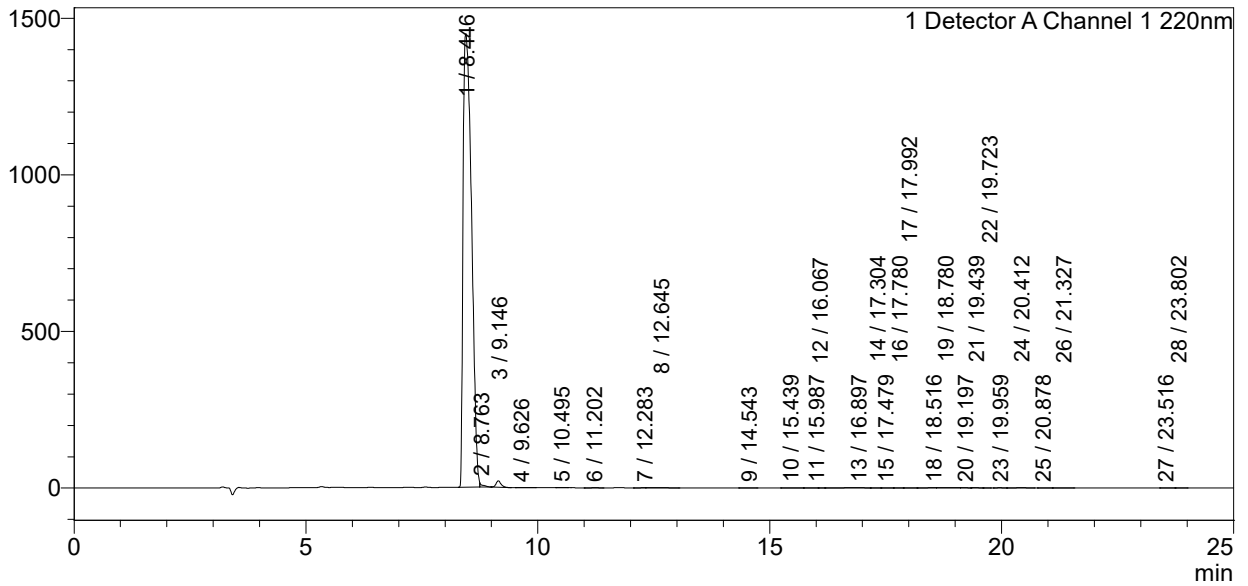

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.446	18230978	1448669	98.307
2	8.763	51805	10692	0.279
3	9.146	151517	20475	0.817
4	9.626	3809	436	0.021
5	10.495	2051	301	0.011
6	11.202	1002	78	0.005
7	12.283	1463	131	0.008
8	12.645	8257	358	0.045
9	14.543	1619	149	0.009
10	15.439	2985	158	0.016
11	15.987	2342	188	0.013
12	16.067	1202	176	0.006
13	16.897	19559	725	0.105
14	17.304	3161	286	0.017

Peak#	Ret. Time	Area	Height	Area%
15	17.479	2692	248	0.015
16	17.780	1619	164	0.009
17	17.992	2361	193	0.013
18	18.516	7064	484	0.038
19	18.780	15961	637	0.086
20	19.197	4383	372	0.024
21	19.439	4512	391	0.024
22	19.723	1726	228	0.009
23	19.959	4403	382	0.024
24	20.412	9393	546	0.051
25	20.878	1360	115	0.007
26	21.327	3065	247	0.017
27	23.516	3648	387	0.020
28	23.802	1018	104	0.005
Total		18544957	1487320	100.000