

Sample Name:β-Amyloid (1-40)  
 Cat No:RP10004  
 Lot No :E9542121B  
 Time Processed :15:24:47  
 Month-Day-Year Processed :05/05/2021


Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Module	Command	Value
0.10	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

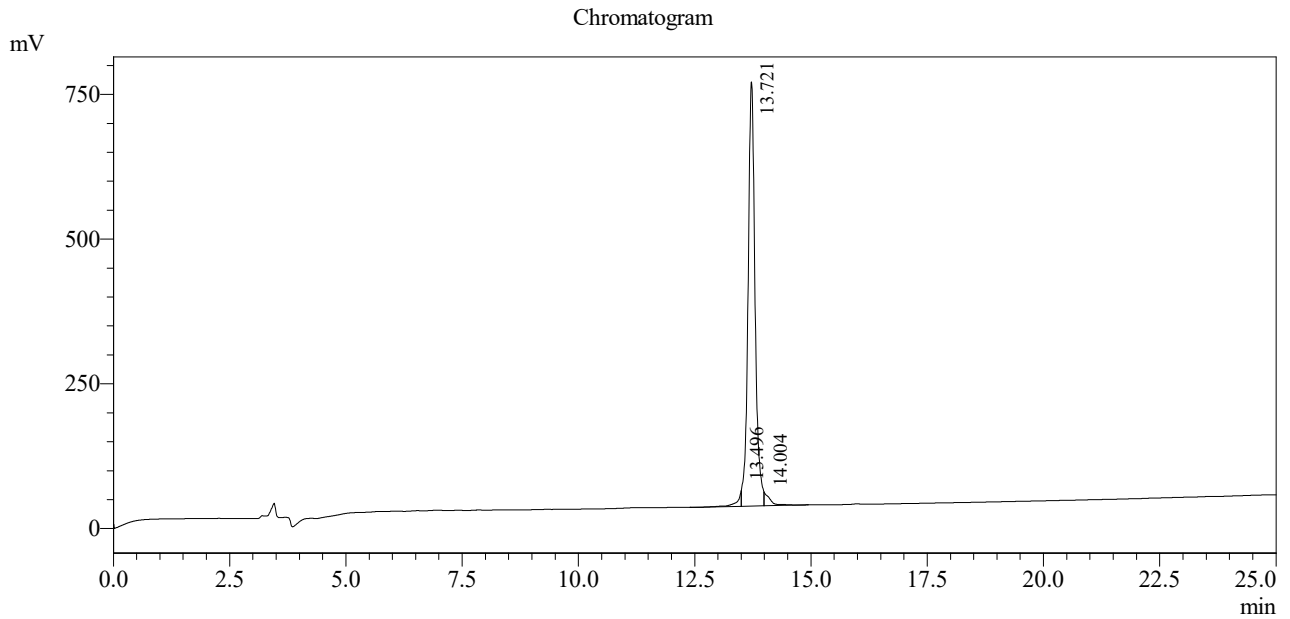

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.496	151288	23868	1.891
2	13.721	7645198	732787	95.576
3	14.004	202622	22534	2.533
Total		7999109	779189	100.000