

Sample Name : $\beta$ -Amyloid (1-42), human  
 Cat No. :RP20527  
 Lot No. :E9790419F  
 Time Processed : 9:03:07  
 Month-Day-Year Processed : 05/27/2019

Pump A : 0.5% Ammonia solution in 100% water (v/v)  
 Pump B : 0.2% Ammonia solution in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
37.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : UniPS 10-300 4.6 x 250 mm

Equipment: GR09010180

Chromatogram

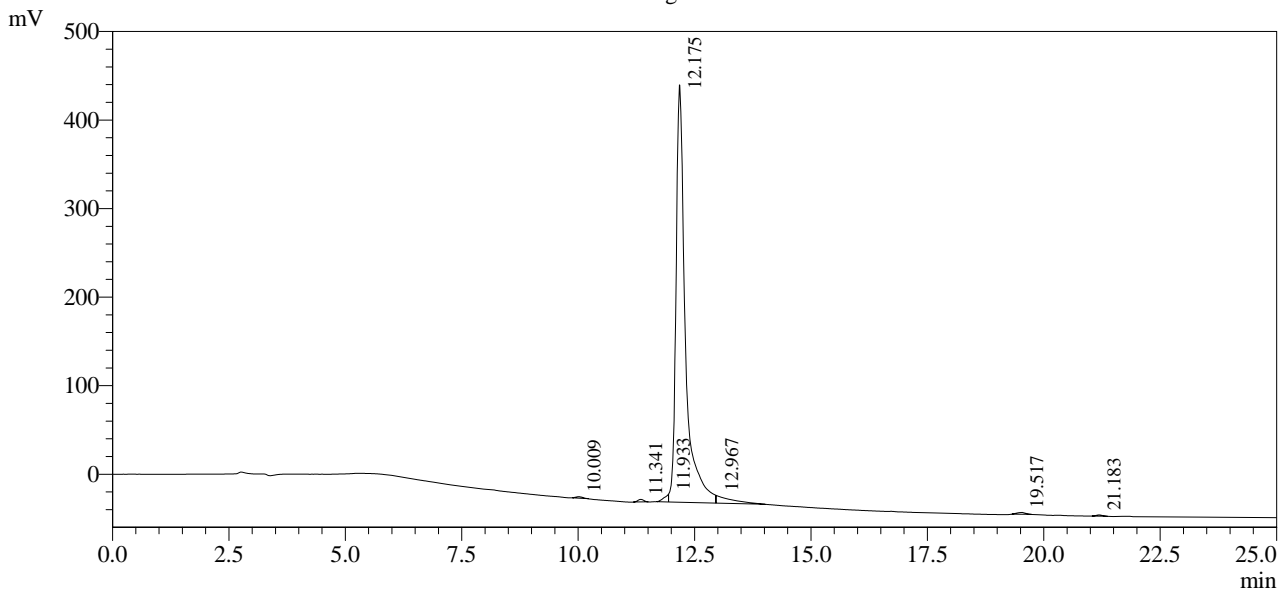

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.009	16315	1588	0.236
2	11.341	25126	2870	0.364
3	11.933	56218	8144	0.813
4	12.175	6580108	471311	95.214
5	12.967	195177	8577	2.824
6	19.517	25485	1965	0.369
7	21.183	12454	1415	0.180
Total		6910882	495869	100.000