

Sample Name : Hepatitis B Virus Core (128-140)
 Cat. No. : RP17313
 Lot. No. : E9674319J
 Time Processed :9:53:05
 Month-Day-Year Processed :10/18/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GR11010440

Chromatogram

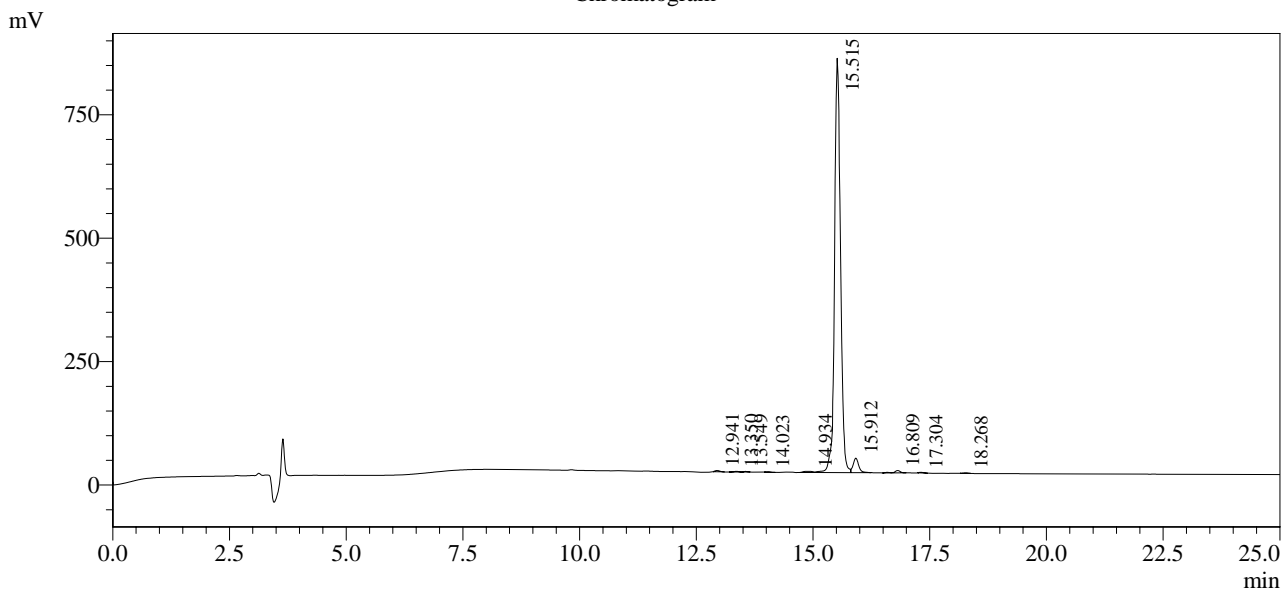

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.941	17705	2581	0.227
2	13.350	9292	1427	0.119
3	13.549	5863	1259	0.075
4	14.023	4434	694	0.057
5	14.934	33877	2288	0.435
6	15.515	7433343	839392	95.340
7	15.912	238354	29317	3.057
8	16.809	41914	4748	0.538
9	17.304	7238	1262	0.093
10	18.268	4655	682	0.060
Total		7796675	883650	100.000