

Sample Name : HA Peptide
 Cat No.: RP11735
 Lot No.: E0366319H
 Time Processed: 2:32:30
 Month-Day-Year Processed: 08/29/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010014

<Chromatogram>

mV

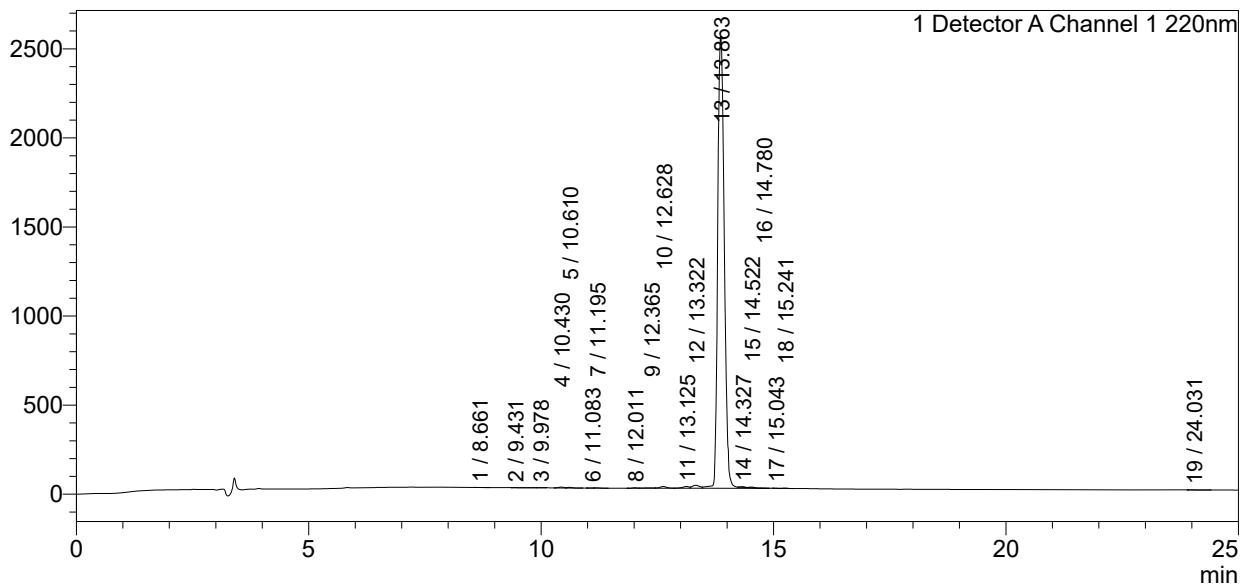

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.661	3490	525	0.014
2	9.431	2904	433	0.011
3	9.978	2698	487	0.011
4	10.430	38751	4867	0.152
5	10.610	27629	3921	0.109
6	11.083	4720	807	0.019
7	11.195	9440	1455	0.037
8	12.011	20068	2981	0.079
9	12.365	37652	2281	0.148
10	12.628	105072	10052	0.413
11	13.125	106394	10102	0.418
12	13.322	184435	16697	0.725
13	13.863	24797421	2538251	97.502
14	14.327	26350	3709	0.104
15	14.522	31804	4188	0.125

Peak#	Ret. Time	Area	Height	Area%
16	14.780	6284	1217	0.025
17	15.043	4358	1018	0.017
18	15.241	18622	2328	0.073
19	24.031	4610	487	0.018
Total		25432700	2605804	100.000