

Sample Name :OVA Peptide (257-264)
Cat No :RP10611
Lot No :PE9881812
Time Processed : 5:38:44
Month-Day-Year Processed : 12/29/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment:GK12010012

<Chromatogram>

mV

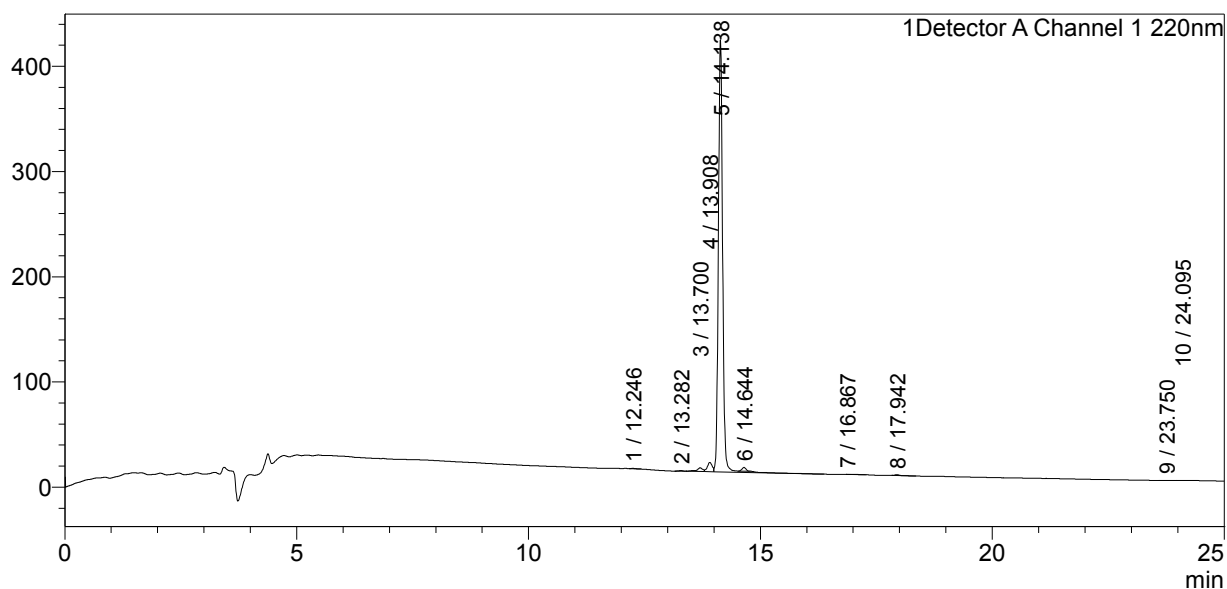

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.246	2033	317	0.074
2	13.282	2959	514	0.107
3	13.700	31020	3454	1.124
4	13.908	63995	8811	2.319
5	14.138	2625431	410624	95.147
6	14.644	21452	3539	0.777
7	16.867	2458	113	0.089
8	17.942	6553	906	0.237
9	23.750	1625	137	0.059
10	24.095	1815	126	0.066
Total		2759341	428542	100.000