

Sample Name :RGD  
 Cat No. : RP20297  
 Lot No. : E8851721F  
 Time Processed : 17:38:06  
 Month-Day-Year Processed : 07/02/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

| Time  | Module     | Command      | Value |
|-------|------------|--------------|-------|
| 0.01  | Pumps      | Pump B Conc. | 5     |
| 25.00 | Pumps      | Pump B Conc. | 65    |
| 25.01 | Pumps      | Pump B Conc. | 95    |
| 27.00 | Pumps      | Pump B Conc. | 95    |
| 27.01 | Pumps      | Pump B Conc. | 5     |
| 32.00 | Pumps      | Pump B Conc. | 5     |
| 32.01 | Controller | Stop         |       |


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment:GK12010012

<Chromatogram>

mV

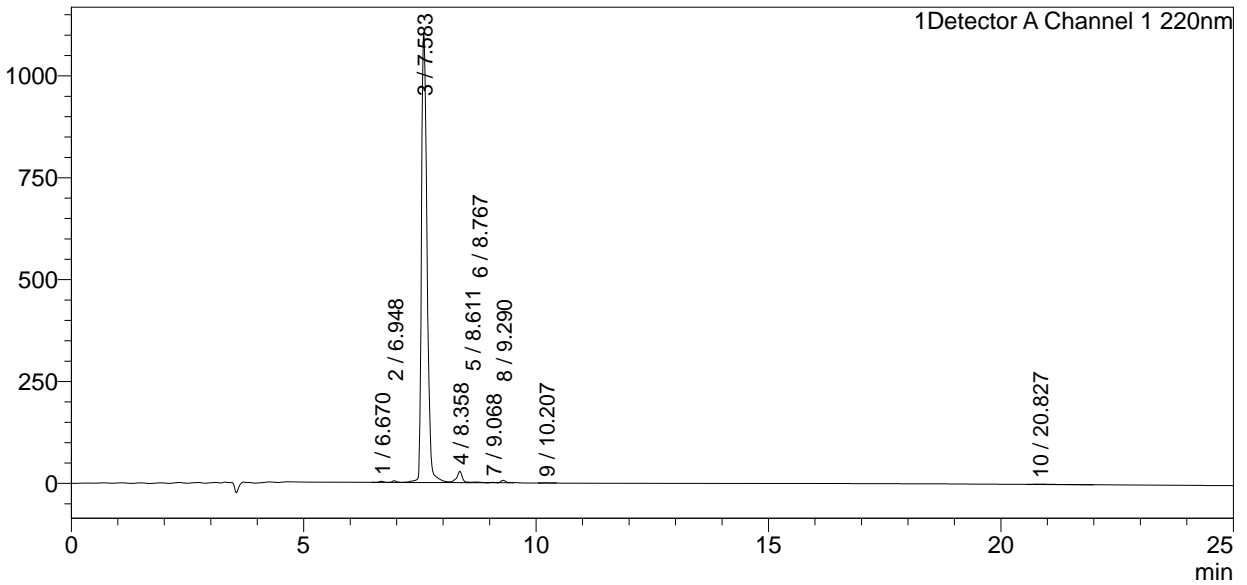

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area    | Height  | Area%   |
|-------|-----------|---------|---------|---------|
| 1     | 6.670     | 19883   | 2870    | 0.209   |
| 2     | 6.948     | 35431   | 4185    | 0.372   |
| 3     | 7.583     | 9130061 | 1098432 | 95.955  |
| 4     | 8.358     | 228114  | 27385   | 2.397   |
| 5     | 8.611     | 14506   | 1564    | 0.152   |
| 6     | 8.767     | 8291    | 1231    | 0.087   |
| 7     | 9.068     | 5164    | 787     | 0.054   |
| 8     | 9.290     | 41482   | 5977    | 0.436   |
| 9     | 10.207    | 4243    | 492     | 0.045   |
| 10    | 20.827    | 27797   | 912     | 0.292   |
| Total |           | 9514972 | 1143834 | 100.000 |