

Sample Name :Gastric Inhibitory Peptide (GIP), human  
 Cat. No. :RP10795  
 Lot. No. : PE2011905  
 Time Processed : 20:11:38  
 Month-Day-Year Processed : 06/03/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	15	
25.00	Pumps	Pump A B.Conc	75	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	15	
40.00	Pumps	Pump A B.Conc	15	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

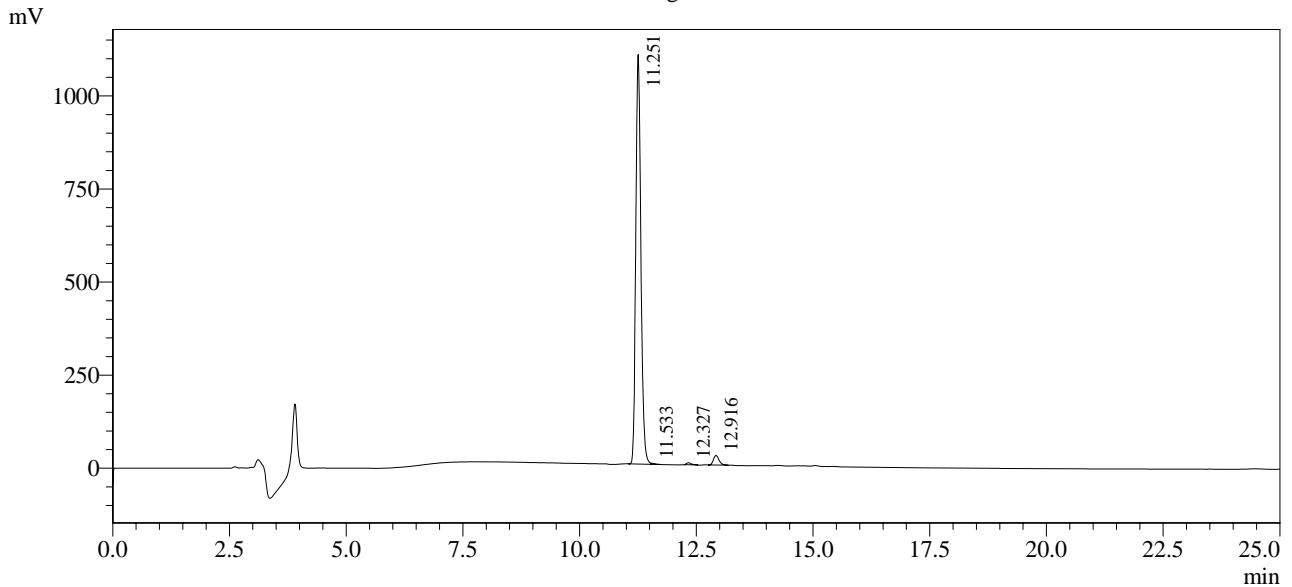

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.251	8376262	1100864	96.888
2	11.533	16085	3088	0.186
3	12.327	37406	5229	0.433
4	12.916	215582	25941	2.494
Total		8645336	1135121	100.000